

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037887.D
 Acq On : 17 Oct 2024 13:37
 Operator : SY/MD
 Sample : P4414-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB	303443	328640	14.40%	2.046%
2	1.532	146	153	167	rVB	267129	317550	13.91%	1.977%
3	2.056	307	316	332	rBV	548909	792451	34.72%	4.933%
4	3.323	708	710	714	rVB3	574	292	0.01%	0.002%
5	3.503	763	766	767	rBV	399	209	0.01%	0.001%
6	3.584	788	791	796	rVB5	761	652	0.03%	0.004%
7	3.612	798	800	802	rBV2	535	289	0.01%	0.002%
8	3.709	827	830	833	rBV3	457	332	0.01%	0.002%
9	3.793	848	856	890	rBV2	72563	219646	9.62%	1.367%
10	4.236	978	994	1029	rBV	375957	956749	41.92%	5.955%
11	4.603	1101	1108	1109	rBV	735	697	0.03%	0.004%
12	4.690	1133	1135	1139	rVB2	710	433	0.02%	0.003%
13	4.712	1139	1142	1146	rBV3	633	387	0.02%	0.002%
14	4.809	1169	1172	1173	rBV2	727	391	0.02%	0.002%
15	4.834	1178	1180	1183	rVB2	418	196	0.01%	0.001%
16	4.870	1187	1191	1194	rBV4	849	625	0.03%	0.004%
17	4.944	1198	1214	1249	rBV2	898093	2282255	100.00%	14.206%
18	5.439	1365	1368	1371	rBV2	898	683	0.03%	0.004%
19	5.526	1383	1395	1422	rBV	644567	1347166	59.03%	8.386%
20	5.934	1521	1522	1524	rBV	620	317	0.01%	0.002%
21	5.979	1524	1536	1567	rVV	496320	1039381	45.54%	6.470%
22	6.249	1617	1620	1622	rBV3	843	566	0.02%	0.004%
23	6.381	1658	1661	1662	rBV2	754	458	0.02%	0.003%
24	6.423	1671	1674	1680	rVB6	818	731	0.03%	0.005%
25	6.445	1680	1681	1683	rBV2	478	241	0.01%	0.002%
26	6.535	1702	1709	1711	rBV4	777	723	0.03%	0.005%
27	6.567	1717	1719	1721	rBV2	297	157	0.01%	0.001%
28	6.606	1727	1731	1733	rBV3	656	347	0.02%	0.002%
29	6.619	1733	1735	1738	rBV3	604	384	0.02%	0.002%
30	6.648	1743	1744	1749	rVB3	609	345	0.02%	0.002%
31	6.673	1749	1752	1754	rVB2	362	219	0.01%	0.001%
32	6.690	1754	1757	1759	rBV3	508	327	0.01%	0.002%
33	6.751	1770	1776	1778	rBV4	914	1054	0.05%	0.007%
34	6.825	1795	1799	1801	rBV3	392	276	0.01%	0.002%
35	6.850	1804	1807	1809	rBV2	315	175	0.01%	0.001%
36	6.866	1809	1812	1814	rBV2	488	357	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037887.D
 Acq On : 17 Oct 2024 13:37
 Operator : SY/MD
 Sample : P4414-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.905	1814	1824	1854	rBV	237953	466763	20.45%	2.905%
38	7.194	1911	1914	1915	rBV2	990	552	0.02%	0.003%
39	7.233	1915	1926	1957	rVV	1001377	1785661	78.24%	11.115%
40	7.548	2015	2024	2046	rBV	153468	293345	12.85%	1.826%
41	7.956	2149	2151	2152	rBV	679	294	0.01%	0.002%
42	8.024	2163	2172	2217	rBV2	207867	502431	22.01%	3.127%
43	8.413	2291	2293	2295	rBV2	839	471	0.02%	0.003%
44	8.497	2316	2319	2323	rBV4	758	553	0.02%	0.003%
45	8.776	2394	2406	2441	rBV	1027698	1730937	75.84%	10.774%
46	9.181	2528	2532	2535	rBV3	744	665	0.03%	0.004%
47	9.278	2560	2562	2566	rVB4	964	538	0.02%	0.003%
48	9.326	2576	2577	2580	rVB	356	169	0.01%	0.001%
49	9.387	2594	2596	2599	rBV3	698	405	0.02%	0.003%
50	9.516	2634	2636	2638	rBV2	556	267	0.01%	0.002%
51	9.558	2646	2649	2651	rBV2	791	500	0.02%	0.003%
52	9.590	2654	2659	2662	rBV2	653	547	0.02%	0.003%
53	9.612	2662	2666	2670	rBV4	908	672	0.03%	0.004%
54	9.644	2670	2676	2679	rVB4	736	795	0.03%	0.005%
55	9.664	2679	2682	2685	rBV2	550	447	0.02%	0.003%
56	9.709	2693	2696	2697	rBV	317	177	0.01%	0.001%
57	9.738	2702	2705	2706	rBV	429	242	0.01%	0.002%
58	9.795	2721	2723	2726	rBV2	395	186	0.01%	0.001%
59	9.844	2735	2738	2740	rBV2	507	201	0.01%	0.001%
60	9.934	2763	2766	2769	rVB3	642	379	0.02%	0.002%
61	9.959	2769	2774	2777	rBV3	620	684	0.03%	0.004%
62	10.017	2790	2792	2796	rBV3	531	384	0.02%	0.002%
63	10.062	2801	2806	2808	rBV	591	575	0.03%	0.004%
64	10.095	2814	2816	2819	rBV	421	315	0.01%	0.002%
65	10.143	2820	2831	2852	rBV	505806	812481	35.60%	5.057%
66	10.464	2928	2931	2934	rVV3	575	360	0.02%	0.002%
67	10.484	2934	2937	2940	rVV3	724	497	0.02%	0.003%
68	10.496	2940	2941	2944	rVV2	547	282	0.01%	0.002%
69	10.519	2944	2948	2954	rVB6	866	760	0.03%	0.005%
70	10.548	2954	2957	2958	rBV	301	173	0.01%	0.001%
71	10.583	2966	2968	2970	rBV2	319	208	0.01%	0.001%
72	10.676	2994	2997	3000	rBV2	466	267	0.01%	0.002%
73	10.718	3006	3010	3014	rBV5	872	769	0.03%	0.005%
74	10.750	3018	3020	3022	rBV	414	262	0.01%	0.002%
75	10.779	3027	3029	3030	rVB	511	158	0.01%	0.001%
76	10.857	3046	3053	3058	rVB6	957	1220	0.05%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037887.D
 Acq On : 17 Oct 2024 13:37
 Operator : SY/MD
 Sample : P4414-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.882	3058	3061	3064	rBV3	715	507	0.02%	0.003%
78	10.895	3064	3065	3067	rBV	348	163	0.01%	0.001%
79	10.930	3074	3076	3079	rVB4	824	379	0.02%	0.002%
80	10.947	3079	3081	3084	rVB2	872	503	0.02%	0.003%
81	10.963	3084	3086	3088	rBV	435	256	0.01%	0.002%
82	11.053	3112	3114	3118	rVB3	356	204	0.01%	0.001%
83	11.101	3125	3129	3131	rBV	507	386	0.02%	0.002%
84	11.120	3133	3135	3137	rBV2	823	500	0.02%	0.003%
85	11.178	3142	3153	3179	rBV	963837	1571940	68.88%	9.785%
86	11.458	3236	3240	3243	rBV3	760	618	0.03%	0.004%
87	11.551	3258	3269	3301	rBV	972542	1581722	69.31%	9.846%
88	11.863	3361	3366	3369	rBV3	1652	1521	0.07%	0.009%
89	11.943	3388	3391	3392	rBV3	786	438	0.02%	0.003%
90	12.085	3433	3435	3438	rBV3	487	256	0.01%	0.002%
91	12.149	3451	3455	3457	rBV	609	564	0.02%	0.004%
92	12.255	3486	3488	3490	rBV2	485	297	0.01%	0.002%
93	12.393	3529	3531	3532	rBV2	476	234	0.01%	0.001%
94	12.509	3564	3567	3574	rVV5	881	789	0.03%	0.005%
95	12.545	3577	3578	3581	rBV2	426	206	0.01%	0.001%
96	12.647	3607	3610	3612	rBV2	447	277	0.01%	0.002%
97	12.776	3648	3650	3652	rBV	650	305	0.01%	0.002%
98	13.114	3753	3755	3756	rBV	560	218	0.01%	0.001%
99	13.352	3827	3829	3831	rBV2	576	326	0.01%	0.002%
100	14.284	4117	4119	4122	rBV3	854	358	0.02%	0.002%




Sum of corrected areas: 16065260

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037887.D
Acq On : 17 Oct 2024 13:37
Operator : SY/MD
Sample : P4414-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

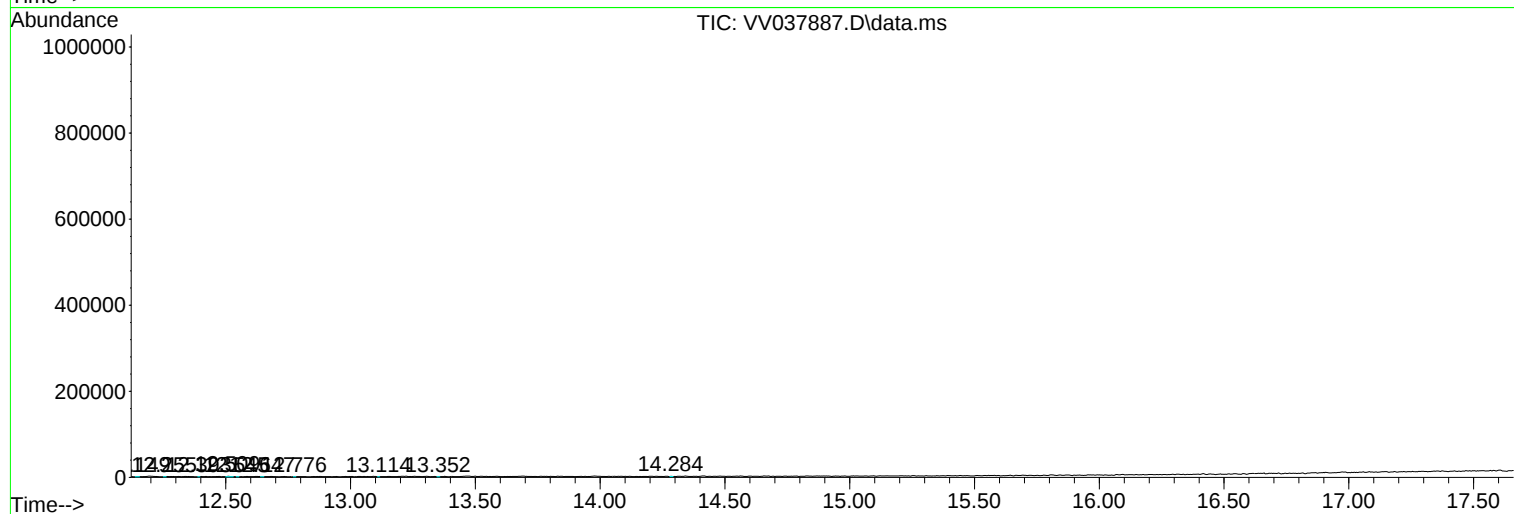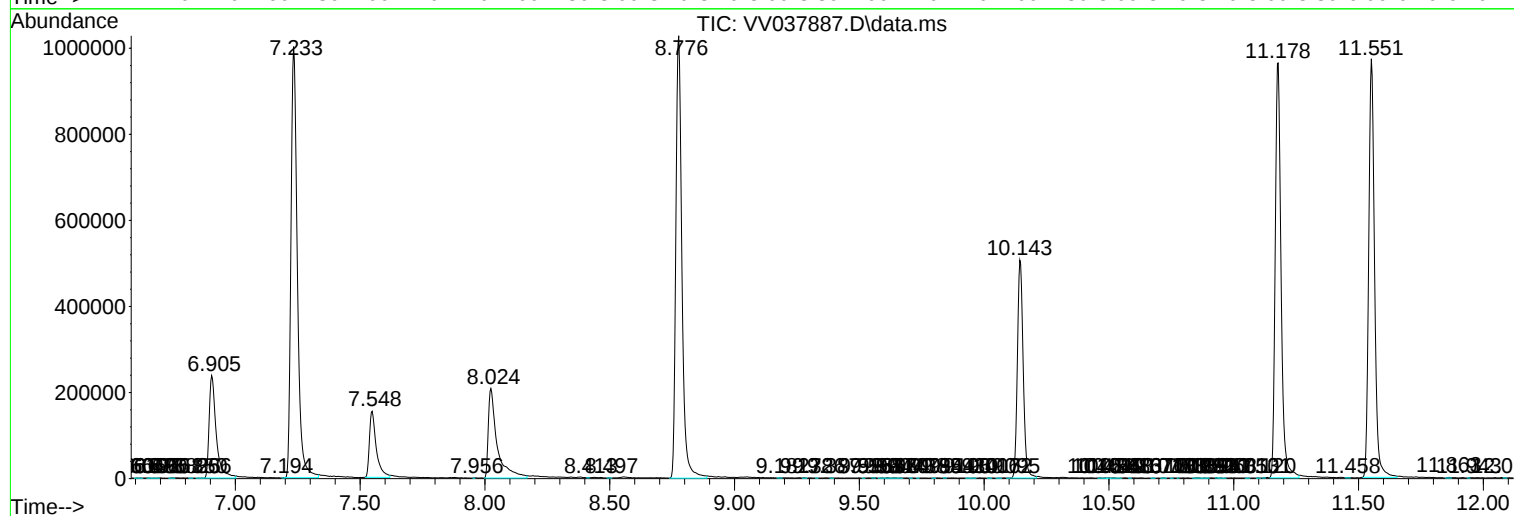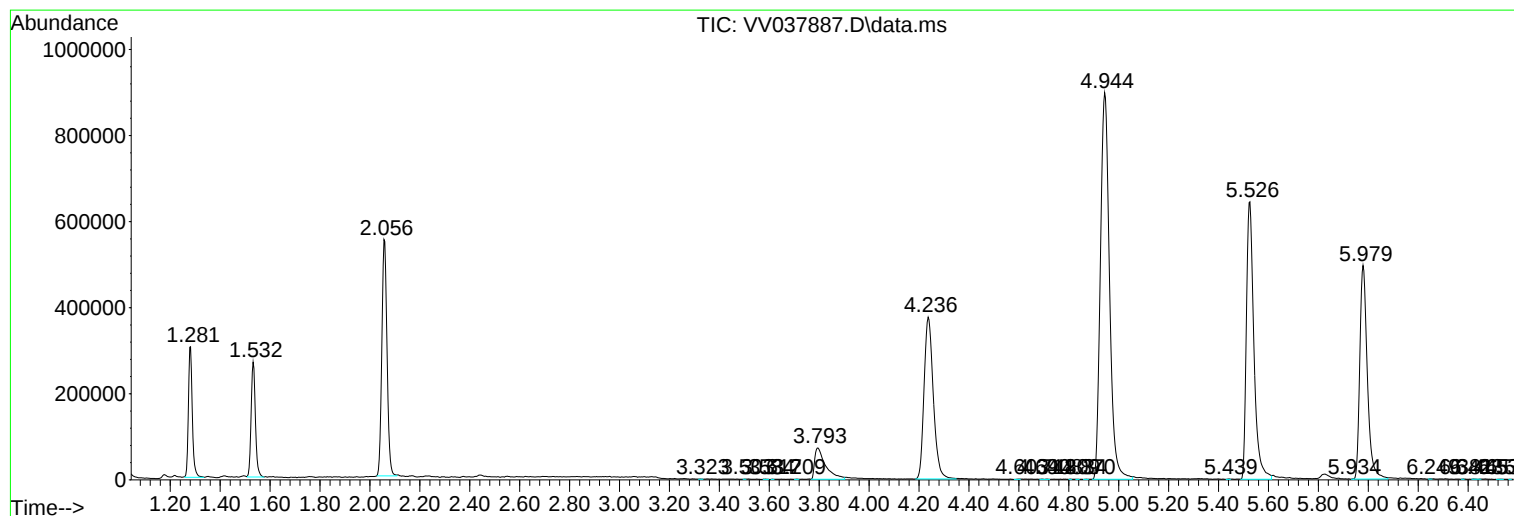

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037887.D
Acq On : 17 Oct 2024 13:37
Operator : SY/MD
Sample : P4414-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037887.D
Acq On : 17 Oct 2024 13:37
Operator : SY/MD
Sample : P4414-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------