
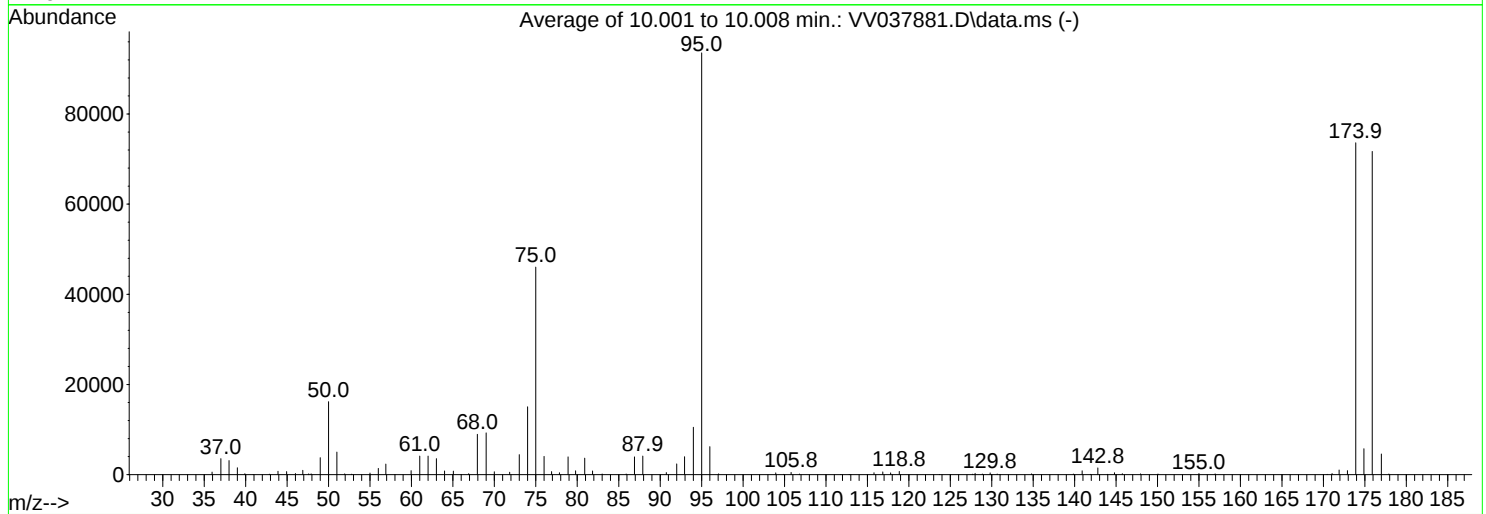


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037881.D
Acq On : 17 Oct 2024 09:01
Operator : SY/MD
Sample : BFB395
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB395

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Fri Oct 18 06:13:48 2024

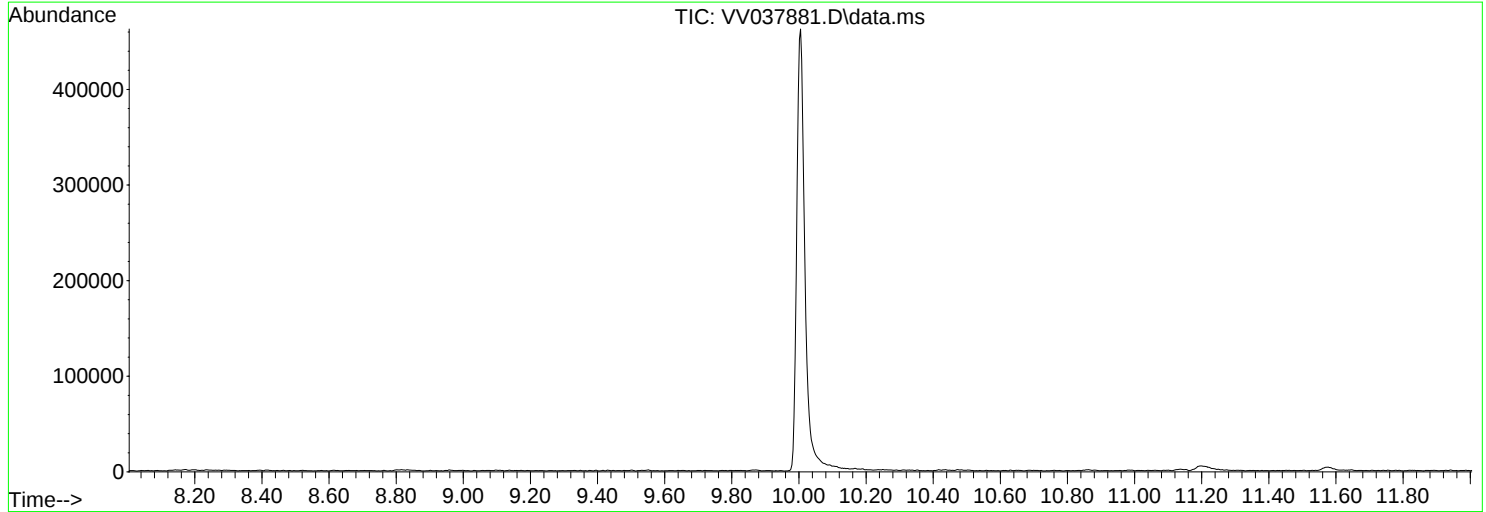

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	16193	PASS
75	95	30	80	49.2	46040	PASS
95	95	100	100	100.0	93563	PASS
96	95	5	9	6.6	6198	PASS
173	174	0.00	2	1.2	905	PASS
174	95	50	120	78.7	73621	PASS
175	174	5	9	7.8	5744	PASS
176	174	95	105	97.4	71693	PASS
177	176	5	10	6.4	4569	PASS

m/z	Abundance
36.00	122.0
40.00	385.0
43.90	490.0

Instrument :
MSVOA_V
ClientSampleId :
BFB395

m/z	Abundance
35.90	785.0
37.00	3439.0
38.00	3171.0
39.00	1519.0
39.90	593.0
42.80	162.0
43.90	1156.0
45.00	709.0
46.00	213.0
46.90	985.0
47.90	571.0
49.00	3715.0
50.00	16504.0
51.00	5273.0
52.00	207.0
52.80	134.0
55.00	335.0
56.00	1573.0
56.90	2474.0
60.00	1011.0
61.00	4334.0
62.00	4218.0
63.00	3513.0
64.00	903.0
65.00	800.0
66.00	101.0
66.90	219.0
68.00	8984.0
69.00	9374.0
70.00	674.0
71.90	629.0
73.00	4412.0
74.00	15590.0
75.00	47480.0
76.00	4148.0
76.90	619.0
77.80	386.0
78.90	3870.0
79.80	867.0
80.90	3943.0
81.90	783.0
83.00	126.0
85.80	163.0
86.90	4268.0
87.90	4162.0
90.70	449.0
92.00	2375.0
92.90	3969.0
94.00	10593.0
95.00	94528.0
96.00	6443.0
97.00	133.0
104.00	415.0
104.90	135.0
105.80	475.0
106.80	185.0
115.80	403.0
116.80	620.0
117.80	493.0
118.80	676.0
127.70	301.0
128.00	319.0
128.90	144.0
129.80	449.0
130.60	107.0
131.00	102.0
134.90	206.0
139.80	119.0
140.90	904.0
141.90	133.0
142.80	1380.0
144.80	491.0
145.70	213.0
148.00	191.0
150.00	142.0
155.00	263.0
157.00	193.0
171.10	245.0
171.90	1063.0
172.90	967.0
173.90	73008.0
174.90	5696.0
175.90	70240.0
177.00	4445.0
177.90	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB395

m/z	Abundance
35.90	720.0
37.00	3649.0
38.00	3208.0
39.00	1607.0
39.90	613.0
42.90	143.0
43.90	1247.0
44.90	680.0
46.00	248.0
46.90	1065.0
49.00	3950.0
50.00	16728.0
51.00	5218.0
52.00	198.0
52.80	118.0
55.00	381.0
56.00	1399.0
56.90	2457.0
59.90	859.0
61.00	4251.0
62.00	4209.0
63.00	3661.0
64.00	836.0
65.10	786.0
66.90	207.0
67.90	9281.0
69.00	9549.0
70.00	682.0
71.80	545.0
73.00	4622.0
74.00	15571.0
75.00	47592.0
76.00	4189.0
76.90	707.0
77.90	419.0
78.90	4097.0
79.80	888.0
80.90	3856.0
81.80	846.0
83.00	148.0
85.90	132.0
86.90	4036.0
87.90	4236.0
90.80	482.0
92.00	2375.0
93.00	4088.0
94.00	10807.0
95.00	97120.0
96.00	6269.0
97.00	197.0
104.00	425.0
104.90	129.0
105.80	521.0
106.80	159.0
112.80	113.0
115.80	412.0
116.80	615.0
117.80	365.0
118.90	737.0
123.70	124.0
128.00	303.0
128.80	170.0
129.80	378.0
130.60	171.0
134.80	187.0
139.90	136.0
140.90	885.0
141.90	103.0
142.80	1559.0
144.00	122.0
144.80	451.0
145.80	244.0
148.00	198.0
150.00	123.0
155.00	248.0
157.00	198.0
170.40	124.0
171.00	247.0
171.90	1022.0
172.90	899.0
173.90	76048.0
174.90	5846.0
175.90	73888.0
177.00	4751.0
177.90	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB395

m/z	Abundance
36.00	611.0
37.00	3561.0
38.00	3016.0
39.00	1484.0
39.90	574.0
40.90	104.0
43.90	1299.0
44.90	621.0
46.00	245.0
46.90	873.0
47.60	509.0
49.00	3680.0
50.00	15347.0
51.00	4508.0
51.90	193.0
52.80	123.0
55.00	388.0
56.00	1144.0
56.90	2148.0
58.00	111.0
59.90	776.0
61.00	3760.0
62.00	3921.0
63.00	3524.0
64.00	740.0
65.10	780.0
66.90	196.0
67.90	8622.0
69.00	8843.0
70.00	573.0
71.80	457.0
73.00	4314.0
74.00	13976.0
75.00	43048.0
76.00	3807.0
76.90	699.0
77.90	467.0
78.90	3854.0
79.80	787.0
80.90	3192.0
81.80	820.0
83.00	127.0
86.00	126.0
86.90	3518.0
87.90	3941.0
90.80	477.0
92.00	2374.0
93.00	3844.0
94.00	10165.0
95.00	89040.0
96.00	5881.0
97.10	248.0
103.90	380.0
105.80	509.0
106.80	133.0
111.80	143.0
113.00	118.0
115.80	425.0
116.90	587.0
117.90	278.0
118.90	735.0
128.00	267.0
128.80	155.0
129.80	321.0
130.70	203.0
134.70	140.0
139.90	138.0
140.90	818.0
142.80	1554.0
143.90	125.0
144.80	369.0
145.70	232.0
147.80	159.0
150.10	127.0
155.00	245.0
156.90	169.0
170.50	124.0
171.00	222.0
171.90	988.0
172.90	850.0
173.90	71808.0
174.90	5689.0
175.90	70952.0
177.00	4512.0
177.90	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB395