

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
 Data File : VV037896.D
 Acq On : 18 Oct 2024 15:37
 Operator : SY/MD
 Sample : P4429-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB8

Quant Time: Oct 18 23:17:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 18 23:14:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	564434	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.777	117	561503	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	252542	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	159120	32.114	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	64.220%		
7) Chloroethane-d5	1.532	69	146131	37.996	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	76.000%		
11) 1,1-Dichloroethene-d2	2.057	65	75921	36.675	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.360%		
21) 2-Butanone-d5	3.793	46	141343	80.089	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	80.090%		
24) Chloroform-d	4.240	84	376868	42.752	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.500%		
26) 1,2-Dichloroethane-d4	4.934	65	226509	43.899	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.800%		
32) Benzene-d6	4.950	84	690331	39.289	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.580%		
36) 1,2-Dichloropropane-d6	5.979	67	234102	41.841	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	83.680%		
41) Toluene-d8	7.236	98	580333	36.425	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	72.840%#		
43) trans-1,3-Dichloroprop...	7.548	79	93512	35.979	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.960%		
47) 2-Hexanone-d5	8.024	63	81353	68.860	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	68.860%		
56) 1,1,2,2-Tetrachloroeth...	10.143	84	263402	40.517	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	81.040%		
66) 1,2-Dichlorobenzene-d4	11.551	152	245105	46.059	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.120%		
Target Compounds					Qvalue	
13) Acetone	2.111	43	44289	25.600	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
Data File : VV037896.D
Acq On : 18 Oct 2024 15:37
Operator : SY/MD
Sample : P4429-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB8

Quant Time: Oct 18 23:17:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 18 23:14:19 2024
Response via : Initial Calibration

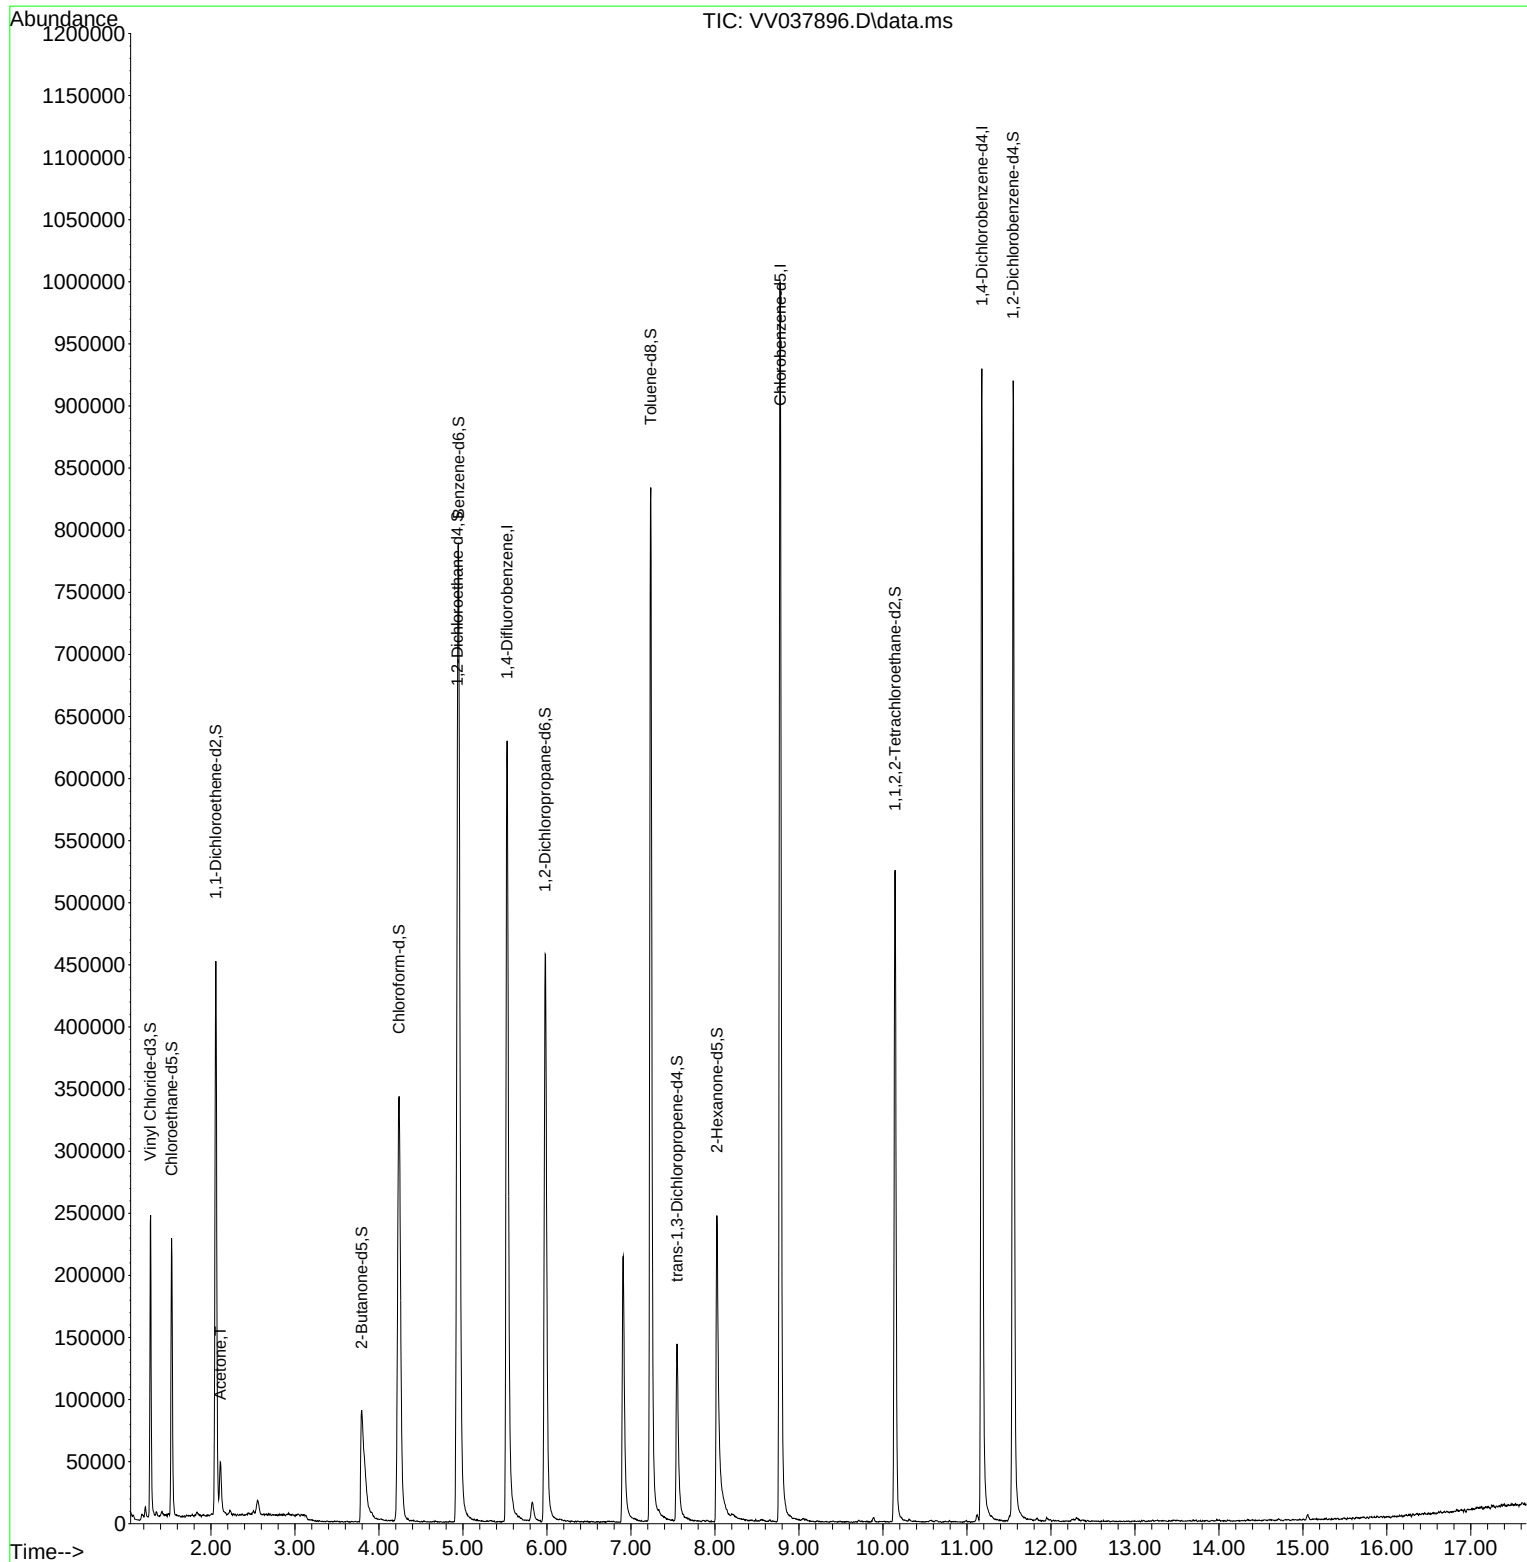

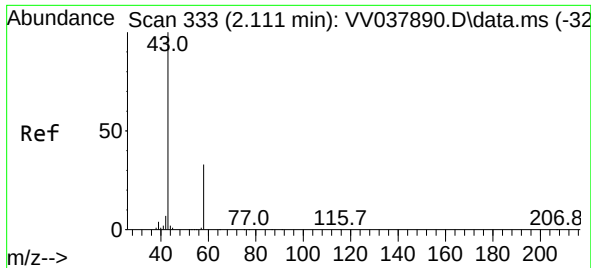

#13

Acetone

Concen: 25.600 ug/L

RT: 2.111 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV037896.D


Acq: 18 Oct 2024 15:37

Instrument :

MSVOA_V

ClientSampleId :

A4EB8

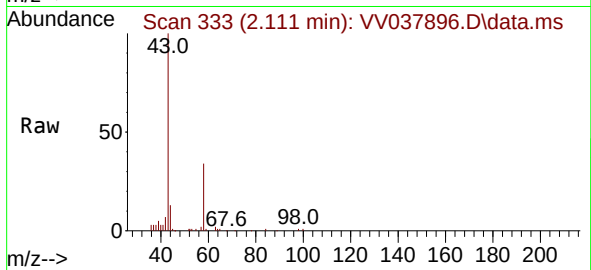

Tgt Ion: 43 Resp: 44289

Ion Ratio Lower Upper

43 100

58 34.0 0.0 66.6

