

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
 Data File : VV037894.D
 Acq On : 18 Oct 2024 14:45
 Operator : SY/MD
 Sample : P4429-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	35	42	51	rBV	13994	23770	1.12%	0.151%
2	1.217	52	55	65	rVV	11024	14542	0.69%	0.092%
3	1.278	67	74	92	rVB	264544	284230	13.42%	1.802%
4	1.532	145	153	167	rVB	238558	283731	13.39%	1.799%
5	2.056	306	316	327	rBV	482674	697544	32.93%	4.424%
6	2.111	328	333	343	rVB	40369	59556	2.81%	0.378%
7	3.429	741	743	748	rVB2	692	495	0.02%	0.003%
8	3.529	772	774	778	rBV4	817	679	0.03%	0.004%
9	3.616	798	801	804	rBV3	681	555	0.03%	0.004%
10	3.654	810	813	815	rBV2	831	587	0.03%	0.004%
11	3.789	846	855	884	rBV	88417	261142	12.33%	1.656%
12	4.236	977	994	1024	rBV	365758	925130	43.67%	5.867%
13	4.609	1106	1110	1113	rVB	677	501	0.02%	0.003%
14	4.764	1153	1158	1160	rBV4	742	609	0.03%	0.004%
15	4.944	1197	1214	1251	rBV2	833599	2118564	100.00%	13.435%
16	5.214	1296	1298	1300	rVB3	983	456	0.02%	0.003%
17	5.294	1319	1323	1324	rBV2	1000	690	0.03%	0.004%
18	5.416	1358	1361	1364	rVB2	750	473	0.02%	0.003%
19	5.522	1381	1394	1429	rBV	659674	1381299	65.20%	8.760%
20	5.821	1477	1487	1506	rBV3	16152	36082	1.70%	0.229%
21	5.979	1523	1536	1570	rBV	478967	1001431	47.27%	6.351%
22	6.358	1649	1654	1655	rBV2	754	661	0.03%	0.004%
23	6.387	1659	1663	1667	rBV3	979	1029	0.05%	0.007%
24	6.506	1697	1700	1705	rVB4	738	614	0.03%	0.004%
25	6.764	1776	1780	1783	rBV6	713	808	0.04%	0.005%
26	6.809	1791	1794	1798	rVB3	622	551	0.03%	0.003%
27	6.860	1804	1810	1813	rVB2	476	476	0.02%	0.003%
28	6.905	1813	1824	1855	rBV	220775	442767	20.90%	2.808%
29	7.095	1881	1883	1889	rBV6	733	836	0.04%	0.005%
30	7.233	1913	1926	1953	rBV	876802	1569521	74.08%	9.953%
31	7.548	2014	2024	2054	rBV	150692	290499	13.71%	1.842%
32	7.857	2116	2120	2123	rVV4	1104	971	0.05%	0.006%
33	7.905	2132	2135	2138	rVB2	1104	700	0.03%	0.004%
34	8.021	2163	2171	2214	rBV2	236631	565038	26.67%	3.583%
35	8.432	2297	2299	2302	rBV3	745	479	0.02%	0.003%
36	8.529	2327	2329	2332	rBV4	1401	925	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
 Data File : VV037894.D
 Acq On : 18 Oct 2024 14:45
 Operator : SY/MD
 Sample : P4429-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.651	2364	2367	2369	rBV4	1077	692	0.03%	0.004%
38	8.702	2380	2383	2386	rBV3	1041	623	0.03%	0.004%
39	8.776	2394	2406	2432	rBV	1047695	1746211	82.42%	11.074%
40	9.156	2522	2524	2527	rVB4	1103	552	0.03%	0.004%
41	9.262	2554	2557	2560	rBV2	924	554	0.03%	0.004%
42	9.284	2560	2564	2567	rBV3	748	817	0.04%	0.005%
43	9.484	2623	2626	2629	rBV2	686	608	0.03%	0.004%
44	9.792	2719	2722	2724	rBV2	879	660	0.03%	0.004%
45	9.853	2736	2741	2745	rVB4	1031	810	0.04%	0.005%
46	9.889	2745	2752	2755	rBV6	2019	2557	0.12%	0.016%
47	9.921	2760	2762	2768	rVB4	693	464	0.02%	0.003%
48	9.972	2773	2778	2780	rBV3	928	663	0.03%	0.004%
49	10.095	2814	2816	2819	rBV3	927	582	0.03%	0.004%
50	10.143	2819	2831	2850	rBV	545078	870297	41.08%	5.519%
51	10.310	2880	2883	2884	rBV2	1436	872	0.04%	0.006%
52	10.603	2970	2974	2979	rVB5	1053	1065	0.05%	0.007%
53	10.628	2979	2982	2991	rBV4	1674	2004	0.09%	0.013%
54	10.828	3039	3044	3049	rBV6	702	719	0.03%	0.005%
55	10.889	3061	3063	3066	rVB	856	489	0.02%	0.003%
56	10.914	3066	3071	3074	rBV	889	718	0.03%	0.005%
57	11.072	3117	3120	3121	rBV2	852	459	0.02%	0.003%
58	11.123	3128	3136	3140	rBV8	4873	6216	0.29%	0.039%
59	11.178	3142	3153	3184	rVV	966554	1565746	73.91%	9.929%
60	11.400	3220	3222	3226	rVB3	970	455	0.02%	0.003%
61	11.464	3239	3242	3244	rBV3	626	498	0.02%	0.003%
62	11.506	3244	3255	3257	rBV6	7015	12032	0.57%	0.076%
63	11.551	3258	3269	3300	rVB	961575	1544389	72.90%	9.794%
64	11.783	3337	3341	3342	rBV3	963	613	0.03%	0.004%
65	11.950	3385	3393	3395	rBV6	2187	2727	0.13%	0.017%
66	12.095	3436	3438	3440	rBV3	834	479	0.02%	0.003%
67	12.249	3480	3486	3489	rBV7	1840	2111	0.10%	0.013%
68	12.300	3496	3502	3504	rBV4	2079	2000	0.09%	0.013%
69	12.442	3542	3546	3550	rBV5	751	802	0.04%	0.005%
70	12.487	3556	3560	3565	rVB4	821	772	0.04%	0.005%
71	12.535	3571	3575	3578	rVB3	1019	831	0.04%	0.005%
72	12.558	3578	3582	3587	rBV4	564	622	0.03%	0.004%
73	12.586	3587	3591	3596	rBV5	1415	1883	0.09%	0.012%
74	12.792	3653	3655	3661	rVV3	738	567	0.03%	0.004%
75	12.824	3661	3665	3667	rVV3	986	630	0.03%	0.004%
76	12.853	3670	3674	3679	rVV6	745	708	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
 Data File : VV037894.D
 Acq On : 18 Oct 2024 14:45
 Operator : SY/MD
 Sample : P4429-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.908	3687	3691	3694	rVB4	638	509	0.02%	0.003%
78	13.181	3772	3776	3778	rBV3	825	594	0.03%	0.004%
79	13.210	3782	3785	3792	rVB7	1692	1871	0.09%	0.012%
80	13.316	3816	3818	3821	rVB	1224	653	0.03%	0.004%
81	13.339	3821	3825	3827	rBV3	1205	907	0.04%	0.006%
82	13.390	3838	3841	3845	rVB4	948	781	0.04%	0.005%
83	13.464	3854	3864	3868	rBV10	2168	4157	0.20%	0.026%
84	13.673	3927	3929	3932	rVV2	934	519	0.02%	0.003%
85	13.696	3933	3936	3943	rVB8	1304	1104	0.05%	0.007%
86	13.815	3970	3973	3978	rBV4	796	811	0.04%	0.005%
87	13.876	3989	3992	3993	rBV	783	505	0.02%	0.003%
88	13.982	4020	4025	4026	rBV3	936	824	0.04%	0.005%
89	14.094	4058	4060	4066	rVB3	568	489	0.02%	0.003%
90	14.204	4091	4094	4096	rBV2	1146	592	0.03%	0.004%
91	14.255	4104	4110	4113	rVB5	988	1135	0.05%	0.007%
92	14.345	4130	4138	4141	rBV6	1618	2121	0.10%	0.013%
93	14.445	4166	4169	4172	rBV3	1292	1068	0.05%	0.007%
94	14.545	4198	4200	4205	rBV3	618	517	0.02%	0.003%
95	14.641	4227	4230	4235	rBV3	929	984	0.05%	0.006%
96	14.680	4239	4242	4246	rVB5	908	748	0.04%	0.005%
97	14.905	4308	4312	4316	rBV7	863	842	0.04%	0.005%
98	15.162	4390	4392	4395	rVB3	1269	509	0.02%	0.003%
99	15.660	4544	4547	4550	rBV3	1661	1226	0.06%	0.008%
100	15.834	4599	4601	4603	rBV3	1374	857	0.04%	0.005%




Sum of corrected areas: 15768761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
Data File : VV037894.D
Acq On : 18 Oct 2024 14:45
Operator : SY/MD
Sample : P4429-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

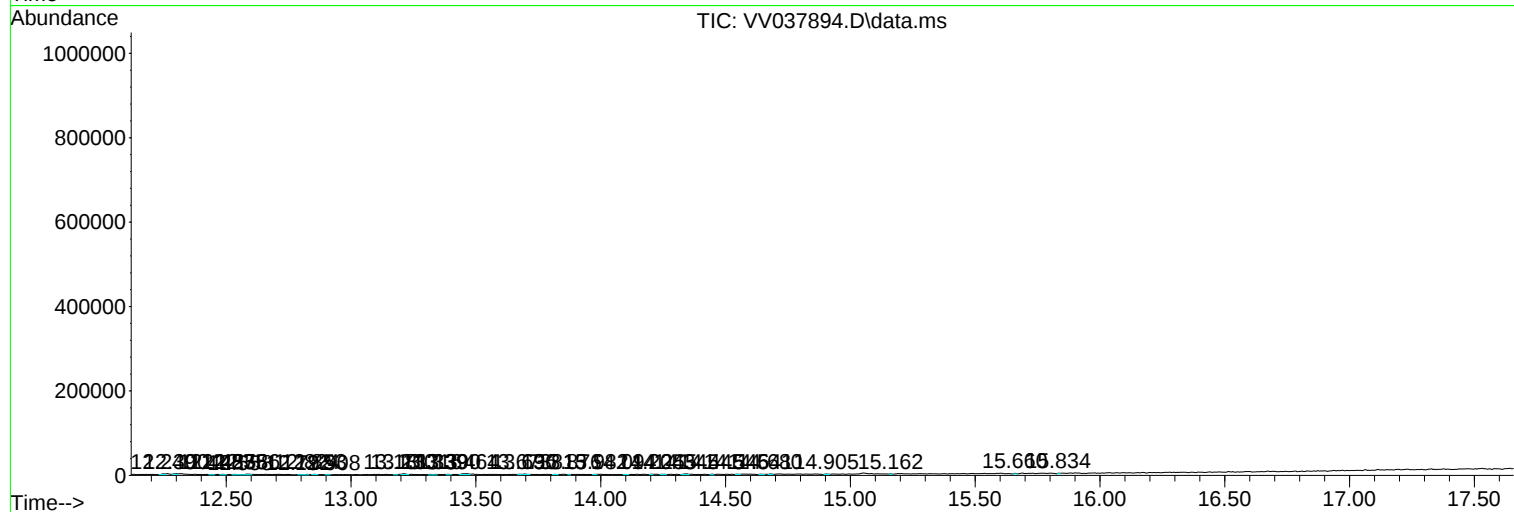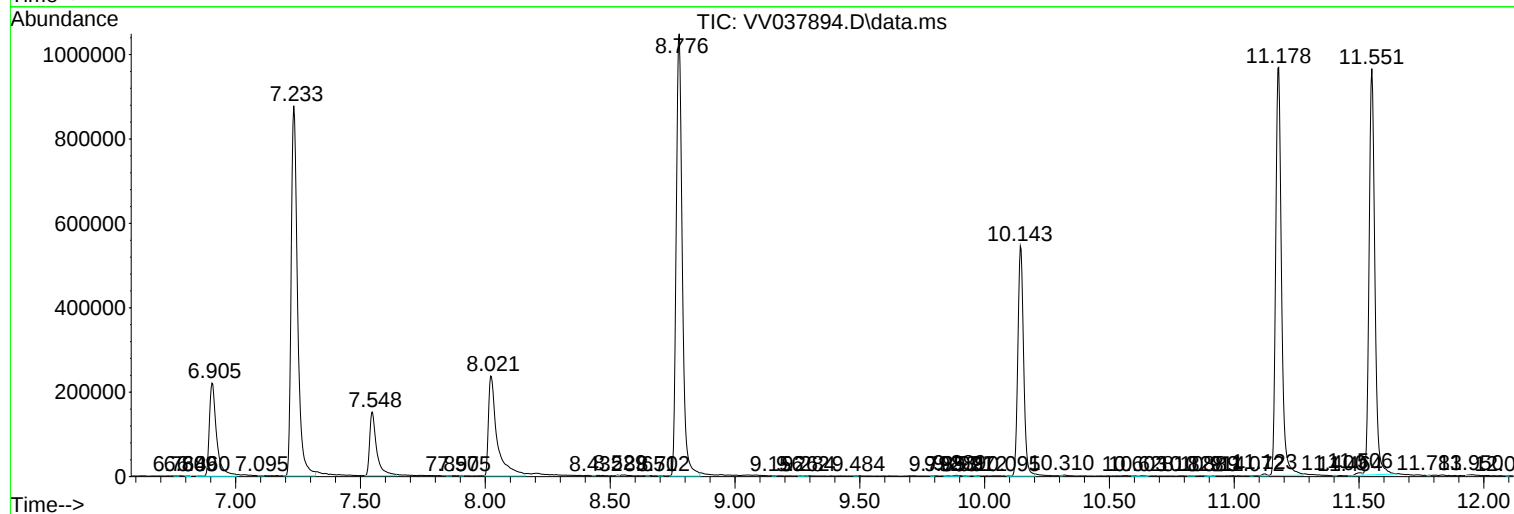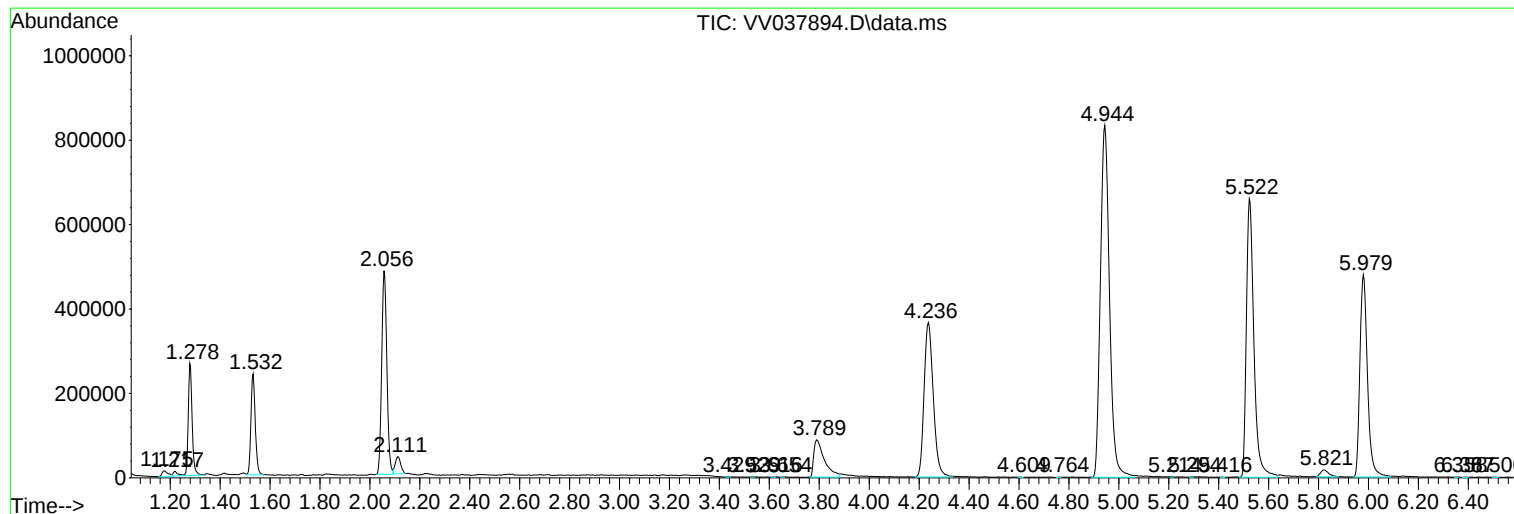

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
Data File : VV037894.D
Acq On : 18 Oct 2024 14:45
Operator : SY/MD
Sample : P4429-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
Data File : VV037894.D
Acq On : 18 Oct 2024 14:45
Operator : SY/MD
Sample : P4429-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------