

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
 Data File : VV037895.D
 Acq On : 18 Oct 2024 15:06
 Operator : SY/MD
 Sample : P4429-23
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rBV	242792	254706	12.86%	1.721%
2	1.532	146	153	168	rVB	223212	259854	13.12%	1.756%
3	2.060	308	317	328	rBV	449997	635075	32.07%	4.291%
4	3.468	752	755	756	rBV	537	310	0.02%	0.002%
5	3.494	761	763	764	rBV	553	215	0.01%	0.001%
6	3.545	776	779	782	rBV2	325	227	0.01%	0.002%
7	3.577	787	789	790	rVB	358	94	0.00%	0.001%
8	3.642	807	809	813	rVB	437	280	0.01%	0.002%
9	3.796	844	857	890	rBV	88100	261960	13.23%	1.770%
10	4.140	962	964	968	rBV2	880	709	0.04%	0.005%
11	4.243	980	996	1027	rBV	341671	864489	43.66%	5.841%
12	4.436	1054	1056	1060	rVB4	1130	640	0.03%	0.004%
13	4.503	1075	1077	1079	rBV3	616	357	0.02%	0.002%
14	4.529	1083	1085	1087	rVB3	503	213	0.01%	0.001%
15	4.545	1087	1090	1091	rBV	582	240	0.01%	0.002%
16	4.564	1094	1096	1101	rBV2	620	481	0.02%	0.003%
17	4.616	1109	1112	1116	rBV3	667	664	0.03%	0.004%
18	4.780	1157	1163	1167	rVB4	731	781	0.04%	0.005%
19	4.805	1167	1171	1172	rBV2	289	225	0.01%	0.002%
20	4.828	1176	1178	1179	rBV	298	97	0.00%	0.001%
21	4.838	1179	1181	1183	rBV2	333	169	0.01%	0.001%
22	4.947	1200	1215	1243	rBV2	776217	1980038	100.00%	13.378%
23	5.278	1316	1318	1326	rBV4	977	924	0.05%	0.006%
24	5.432	1363	1366	1367	rBV2	467	291	0.01%	0.002%
25	5.458	1372	1374	1376	rBV2	402	188	0.01%	0.001%
26	5.474	1376	1379	1380	rBV4	500	280	0.01%	0.002%
27	5.529	1385	1396	1439	rVV	623274	1309755	66.15%	8.849%
28	5.982	1526	1537	1563	rBV	457147	942861	47.62%	6.370%
29	6.326	1642	1644	1646	rBV	511	266	0.01%	0.002%
30	6.416	1667	1672	1675	rBV2	916	863	0.04%	0.006%
31	6.442	1678	1680	1682	rVB2	655	250	0.01%	0.002%
32	6.529	1706	1707	1713	rVB3	522	284	0.01%	0.002%
33	6.555	1713	1715	1717	rVB	353	188	0.01%	0.001%
34	6.580	1717	1723	1727	rBV3	1414	1154	0.06%	0.008%
35	6.619	1731	1735	1736	rBV	577	295	0.01%	0.002%
36	6.629	1736	1738	1739	rVB2	376	95	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
 Data File : VV037895.D
 Acq On : 18 Oct 2024 15:06
 Operator : SY/MD
 Sample : P4429-23
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.674	1749	1752	1755	rVB3	665	395	0.02%	0.003%
38	6.702	1755	1761	1764	rBV6	753	963	0.05%	0.007%
39	6.725	1766	1768	1771	rBV2	459	238	0.01%	0.002%
40	6.780	1783	1785	1788	rBV2	574	300	0.02%	0.002%
41	6.821	1795	1798	1800	rBV2	617	303	0.02%	0.002%
42	6.860	1807	1810	1811	rBV2	357	152	0.01%	0.001%
43	6.908	1814	1825	1864	rBV	212318	424591	21.44%	2.869%
44	7.236	1916	1927	1952	rBV	824934	1472655	74.38%	9.950%
45	7.551	2016	2025	2056	rBV2	144427	277520	14.02%	1.875%
46	7.944	2143	2147	2149	rBV4	850	616	0.03%	0.004%
47	7.956	2149	2151	2155	rVB3	931	590	0.03%	0.004%
48	8.024	2164	2172	2203	rBV2	245712	574228	29.00%	3.880%
49	8.735	2390	2393	2394	rBV2	821	373	0.02%	0.003%
50	8.776	2395	2406	2439	rVV	1006853	1679928	84.84%	11.350%
51	9.156	2522	2524	2526	rBV2	463	139	0.01%	0.001%
52	9.313	2568	2573	2574	rBV4	836	528	0.03%	0.004%
53	9.355	2582	2586	2589	rBV3	1307	1199	0.06%	0.008%
54	9.390	2594	2597	2599	rBV2	579	365	0.02%	0.002%
55	9.423	2605	2607	2609	rVB2	378	157	0.01%	0.001%
56	9.442	2611	2613	2617	rVB3	603	291	0.01%	0.002%
57	9.464	2617	2620	2621	rBV	234	123	0.01%	0.001%
58	9.474	2621	2623	2625	rBV2	323	172	0.01%	0.001%
59	9.493	2627	2629	2631	rVV2	586	377	0.02%	0.003%
60	9.519	2634	2637	2643	rVB4	537	475	0.02%	0.003%
61	9.554	2646	2648	2651	rBV2	559	348	0.02%	0.002%
62	9.641	2673	2675	2676	rVB	766	173	0.01%	0.001%
63	9.654	2676	2679	2680	rBV	316	163	0.01%	0.001%
64	9.664	2680	2682	2685	rVB2	472	208	0.01%	0.001%
65	9.683	2685	2688	2690	rBV2	159	108	0.01%	0.001%
66	9.696	2690	2692	2693	rBV	508	222	0.01%	0.001%
67	9.715	2693	2698	2706	rVB6	1604	2201	0.11%	0.015%
68	9.754	2706	2710	2715	rBV4	667	623	0.03%	0.004%
69	9.776	2715	2717	2719	rBV2	681	416	0.02%	0.003%
70	9.808	2724	2727	2729	rVB3	658	331	0.02%	0.002%
71	9.825	2729	2732	2734	rBV4	638	400	0.02%	0.003%
72	9.866	2738	2745	2746	rBV2	980	758	0.04%	0.005%
73	9.882	2746	2750	2753	rBV5	2277	2270	0.11%	0.015%
74	9.943	2765	2769	2771	rBV2	436	293	0.01%	0.002%
75	9.995	2782	2785	2787	rBV3	641	358	0.02%	0.002%
76	10.059	2803	2805	2808	rBV2	506	224	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
 Data File : VV037895.D
 Acq On : 18 Oct 2024 15:06
 Operator : SY/MD
 Sample : P4429-23
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.095	2813	2816	2818	rBV2	402	226	0.01%	0.002%
78	10.146	2818	2832	2856	rBV	539284	868930	43.88%	5.871%
79	10.413	2913	2915	2917	rBV	436	195	0.01%	0.001%
80	10.477	2932	2935	2939	rBV2	507	382	0.02%	0.003%
81	10.532	2950	2952	2955	rBV	529	406	0.02%	0.003%
82	10.767	3023	3025	3027	rBV2	270	132	0.01%	0.001%
83	10.783	3029	3030	3034	rVV2	473	277	0.01%	0.002%
84	10.828	3040	3044	3046	rBV2	385	263	0.01%	0.002%
85	10.841	3046	3048	3051	rVB	564	273	0.01%	0.002%
86	10.870	3055	3057	3058	rBV	564	286	0.01%	0.002%
87	10.947	3079	3081	3083	rBV3	560	323	0.02%	0.002%
88	10.976	3087	3090	3091	rBV	649	348	0.02%	0.002%
89	11.079	3118	3122	3125	rBV3	648	598	0.03%	0.004%
90	11.124	3127	3136	3141	rBV10	4794	7251	0.37%	0.049%
91	11.178	3143	3153	3180	rVV	927500	1496227	75.57%	10.109%
92	11.551	3259	3269	3298	rBV	920691	1455878	73.53%	9.836%
93	11.931	3385	3387	3388	rBV2	1169	523	0.03%	0.004%
94	12.982	3711	3714	3716	rBV3	738	447	0.02%	0.003%
95	13.046	3732	3734	3736	rBV2	692	386	0.02%	0.003%
96	13.078	3741	3744	3745	rBV2	636	372	0.02%	0.003%
97	13.194	3777	3780	3781	rBV	850	389	0.02%	0.003%
98	13.262	3798	3801	3804	rBV3	847	739	0.04%	0.005%
99	13.548	3887	3890	3892	rBV3	908	474	0.02%	0.003%
100	13.609	3906	3909	3910	rBV3	815	422	0.02%	0.003%




Sum of corrected areas: 14801039

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
Data File : VV037895.D
Acq On : 18 Oct 2024 15:06
Operator : SY/MD
Sample : P4429-23
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

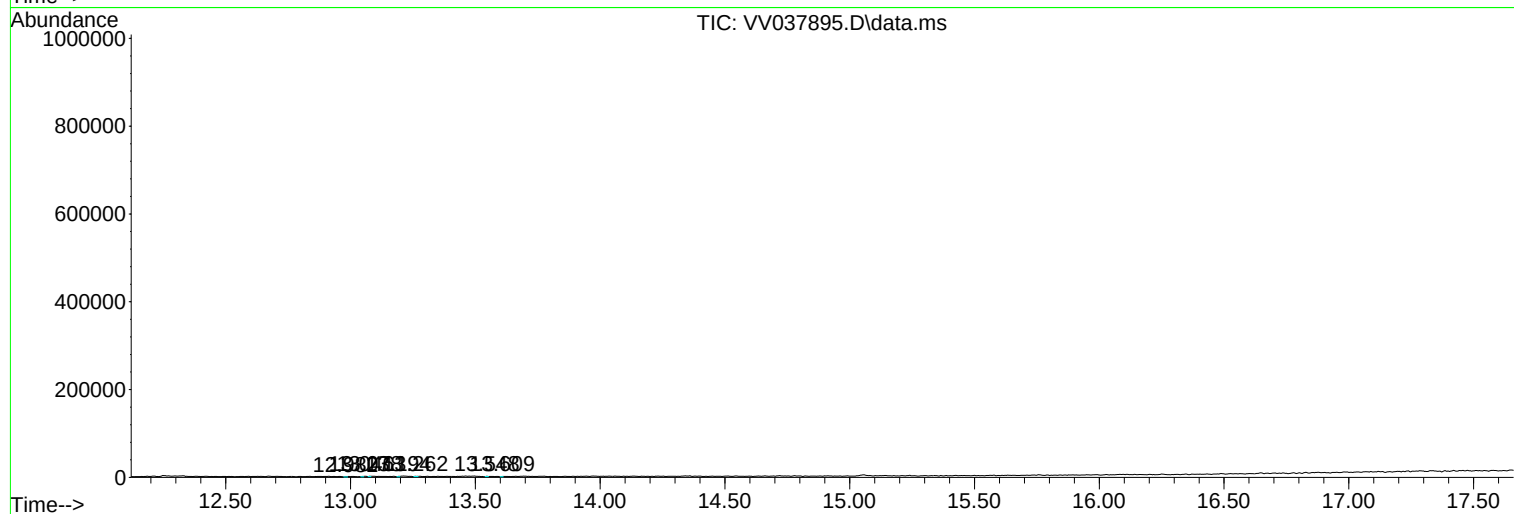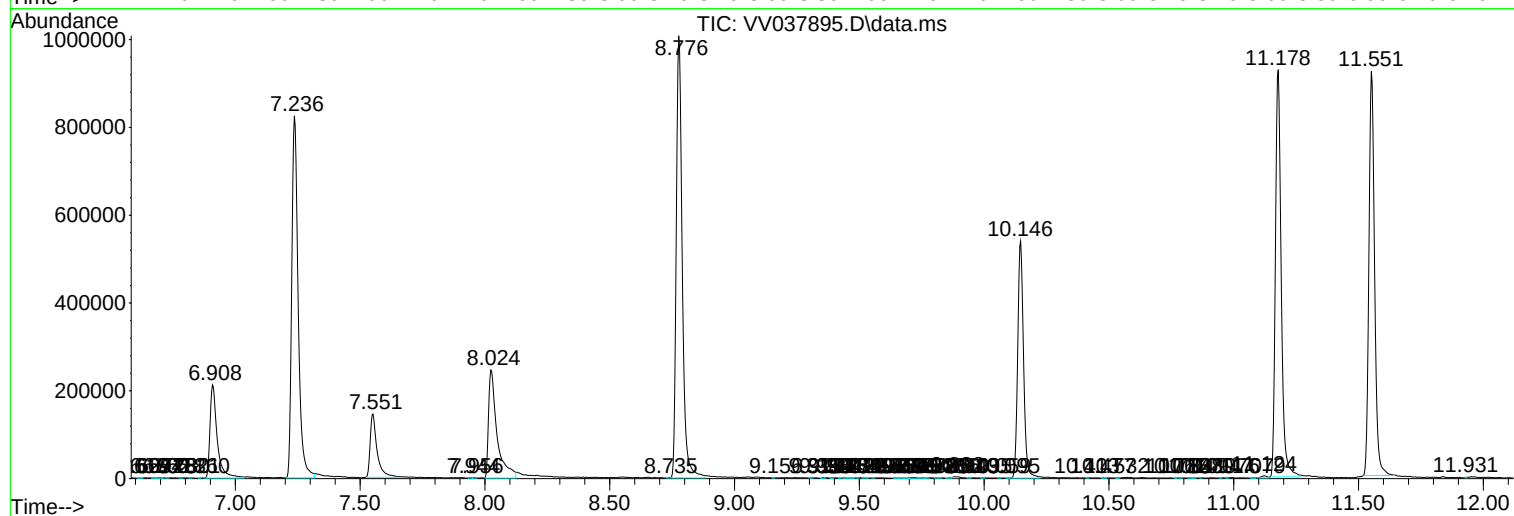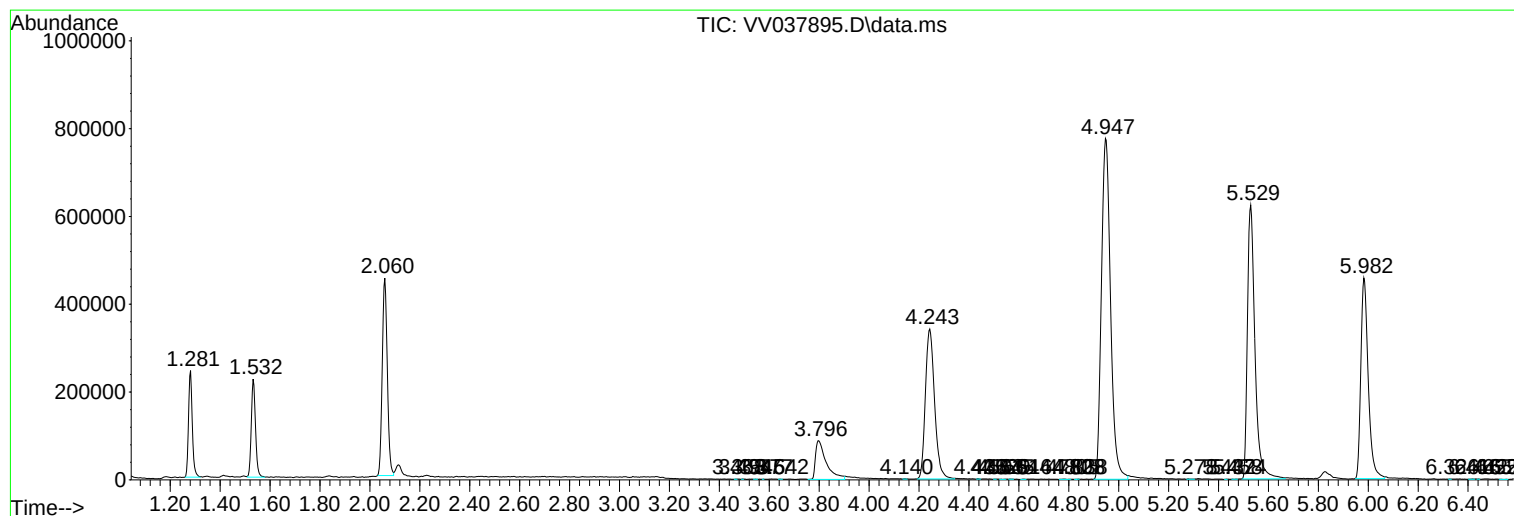

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
Data File : VV037895.D
Acq On : 18 Oct 2024 15:06
Operator : SY/MD
Sample : P4429-23
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
Data File : VV037895.D
Acq On : 18 Oct 2024 15:06
Operator : SY/MD
Sample : P4429-23
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------