
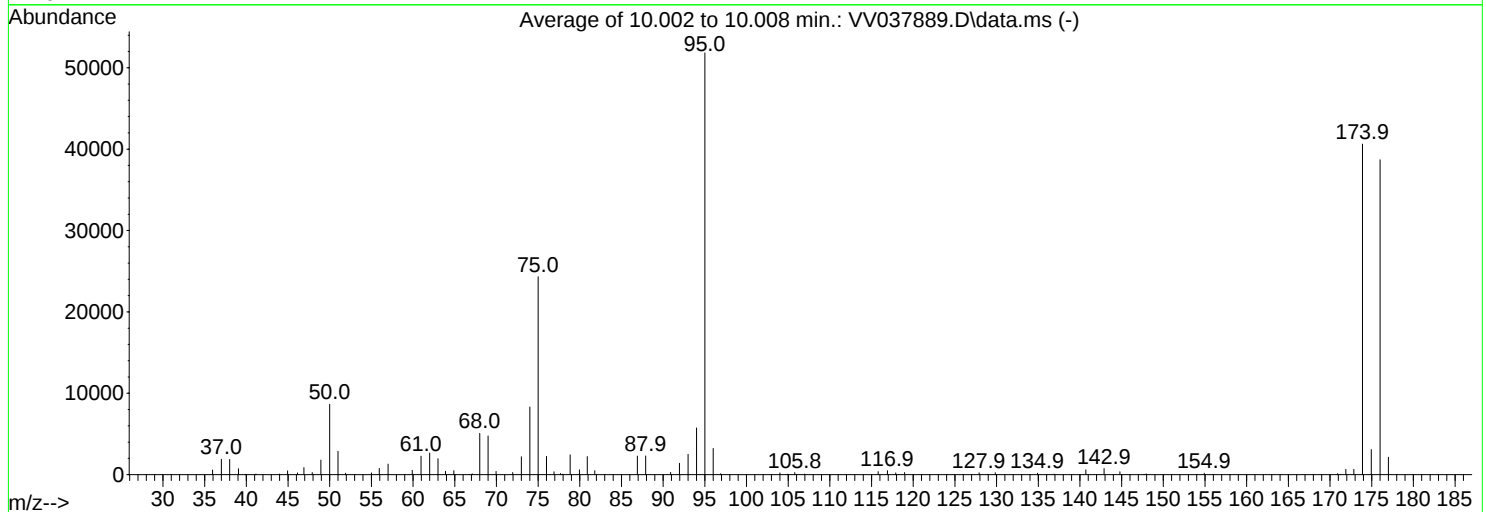


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101824\
Data File : VV037889.D
Acq On : 18 Oct 2024 09:04
Operator : SY/MD
Sample : BFB396
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB396

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Fri Oct 18 23:14:19 2024

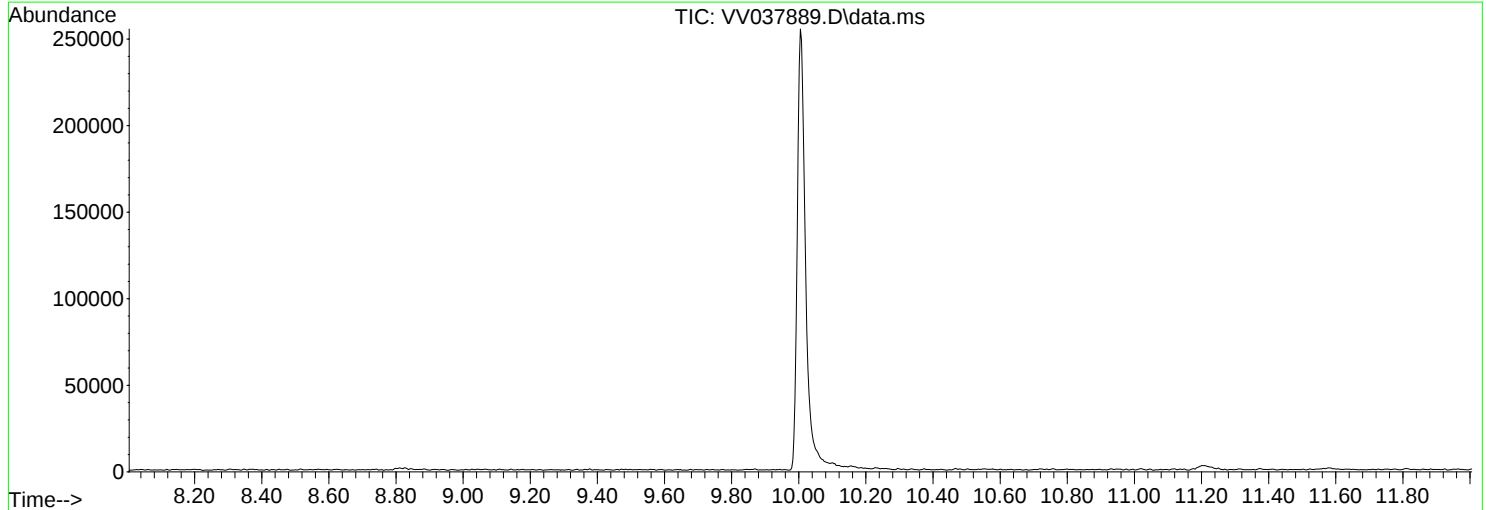

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	8661	PASS
75	95	30	80	46.9	24315	PASS
95	95	100	100	100.0	51832	PASS
96	95	5	9	6.2	3234	PASS
173	174	0.00	2	1.6	652	PASS
174	95	50	120	78.4	40624	PASS
175	174	5	9	7.6	3089	PASS
176	174	95	105	95.3	38696	PASS
177	176	5	10	5.5	2146	PASS

m/z	Abundance
39.90	459.0
43.90	591.0

Instrument :
MSVOA_V
ClientSampleId :
BFB396

m/z	Abundance
35.90	576.0
37.00	1782.0
38.00	1777.0
39.10	825.0
39.90	496.0
41.10	129.0
44.00	677.0
45.00	526.0
46.10	173.0
46.90	688.0
47.90	238.0
48.90	1860.0
50.00	8306.0
51.00	2715.0
51.90	203.0
55.00	219.0
55.90	752.0
57.00	1316.0
59.90	453.0
60.90	2165.0
62.00	2260.0
63.00	1961.0
63.90	502.0
64.90	408.0
67.10	150.0
68.00	5158.0
69.00	4444.0
69.90	436.0
71.90	319.0
73.00	1930.0
74.00	8216.0
75.00	23688.0
76.00	2360.0
76.90	281.0
77.70	208.0
78.90	2417.0
80.00	565.0
80.90	2111.0
81.80	527.0
86.90	2247.0
87.90	2335.0
90.90	324.0
91.90	1363.0
93.00	2528.0
94.00	5380.0
95.00	49728.0
96.00	3222.0
104.00	215.0
105.80	299.0
115.80	364.0
116.90	419.0
117.90	232.0
118.90	234.0
127.90	246.0
128.90	107.0
129.80	245.0
134.90	150.0
136.90	106.0
140.70	620.0
142.90	673.0
144.80	367.0
148.00	151.0
155.00	208.0
171.00	140.0
171.90	628.0
172.80	688.0
173.90	37408.0
174.90	2825.0
176.00	35864.0
177.00	2159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB396

m/z	Abundance
35.90	615.0
37.00	1952.0
38.00	1924.0
39.10	740.0
39.90	494.0
41.20	100.0
44.00	649.0
44.90	492.0
46.20	231.0
46.90	916.0
47.90	274.0
49.00	1831.0
50.00	8967.0
51.00	3018.0
51.90	176.0
55.00	235.0
56.00	788.0
57.00	1343.0
59.90	558.0
61.00	2344.0
62.00	2784.0
63.00	2041.0
63.90	432.0
64.90	484.0
67.10	151.0
68.00	5304.0
69.00	4945.0
69.90	420.0
71.90	252.0
73.00	2297.0
74.00	8710.0
75.00	25024.0
76.00	2287.0
76.90	342.0
77.70	188.0
78.80	2518.0
80.00	636.0
80.90	2274.0
81.80	493.0
86.90	2404.0
87.90	2451.0
90.90	306.0
91.90	1421.0
93.00	2601.0
94.00	5904.0
95.00	53792.0
96.00	3287.0
96.90	151.0
104.00	236.0
104.90	106.0
105.80	250.0
106.90	124.0
115.80	405.0
116.90	517.0
117.90	221.0
119.00	248.0
127.90	258.0
129.80	266.0
134.90	187.0
136.90	108.0
140.70	593.0
142.90	790.0
144.80	376.0
147.90	135.0
154.90	165.0
170.90	112.0
171.20	108.0
171.90	671.0
172.90	667.0
173.90	42224.0
175.00	3206.0
176.00	40104.0
177.00	2192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB396

m/z	Abundance
36.00	542.0
37.00	1958.0
38.00	1887.0
39.00	640.0
39.90	503.0
44.00	660.0
44.90	383.0
46.20	249.0
46.90	1014.0
47.90	281.0
49.00	1685.0
50.00	8709.0
51.00	2871.0
51.90	168.0
55.00	201.0
56.00	781.0
57.00	1231.0
59.90	613.0
61.00	2265.0
62.00	2904.0
63.00	1896.0
63.90	315.0
64.90	598.0
66.80	142.0
68.00	4767.0
69.00	4910.0
70.00	338.0
72.00	229.0
73.00	2375.0
74.00	8008.0
75.00	24232.0
76.00	2072.0
76.90	430.0
77.90	192.0
78.90	2411.0
79.90	597.0
80.90	2259.0
81.80	463.0
86.90	2214.0
87.90	2132.0
90.90	224.0
92.00	1398.0
93.00	2352.0
94.00	5954.0
95.00	51976.0
96.00	3194.0
96.90	198.0
104.00	211.0
104.90	102.0
105.80	220.0
107.00	112.0
115.80	370.0
116.90	527.0
117.90	225.0
119.00	293.0
127.90	228.0
129.90	213.0
134.90	181.0
140.70	547.0
142.90	784.0
144.80	346.0
147.70	105.0
154.80	166.0
157.00	116.0
170.80	127.0
171.90	663.0
172.90	600.0
173.90	42240.0
175.00	3237.0
176.00	40120.0
177.00	2087.0

Instrument :
MSVOA_V
ClientSampleId :
BFB396