

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102224\
 Data File : VV037910.D
 Acq On : 22 Oct 2024 14:41
 Operator : SY/MD
 Sample : VIBLK390
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK390

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101624WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV037910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	87	rBV	96382	108323	12.31%	1.428%
2	1.529	145	152	167	rVB	97119	115072	13.08%	1.517%
3	2.053	305	315	330	rVV	188817	275267	31.29%	3.628%
4	2.442	427	436	450	rVB4	6202	11628	1.32%	0.153%
5	3.799	844	858	895	rBV3	99802	354286	40.27%	4.670%
6	4.243	977	996	1022	rBV	141492	386260	43.90%	5.091%
7	4.950	1203	1216	1255	rBV2	317328	846045	96.16%	11.152%
8	5.529	1386	1396	1429	rBV	289977	646998	73.54%	8.528%
9	5.834	1478	1491	1500	rBV	4076	9317	1.06%	0.123%
10	5.982	1522	1537	1566	rBV2	184500	417440	47.45%	5.502%
11	6.915	1816	1827	1855	rBV	69533	164169	18.66%	2.164%
12	7.239	1916	1928	1951	rBV	327906	634134	72.08%	8.359%
13	7.561	2019	2028	2051	rBV2	38384	89569	10.18%	1.181%
14	8.024	2163	2172	2214	rBV	342948	841219	95.61%	11.088%
15	8.362	2269	2277	2289	rVB4	8831	15777	1.79%	0.208%
16	8.780	2396	2407	2436	rBV	484736	879825	100.00%	11.597%
17	9.085	2495	2502	2521	rVB5	6355	12423	1.41%	0.164%
18	10.146	2819	2832	2854	rBV	155935	266072	30.24%	3.507%
19	11.181	3141	3154	3182	rBV	460028	818088	92.98%	10.783%
20	11.554	3259	3270	3301	rBV	357912	655729	74.53%	8.643%
21	13.204	3771	3783	3801	rBV4	17705	38893	4.42%	0.513%




Sum of corrected areas: 7586534

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102224\
Data File : VV037910.D
Acq On : 22 Oct 2024 14:41
Operator : SY/MD
Sample : VIBLK390
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK390

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

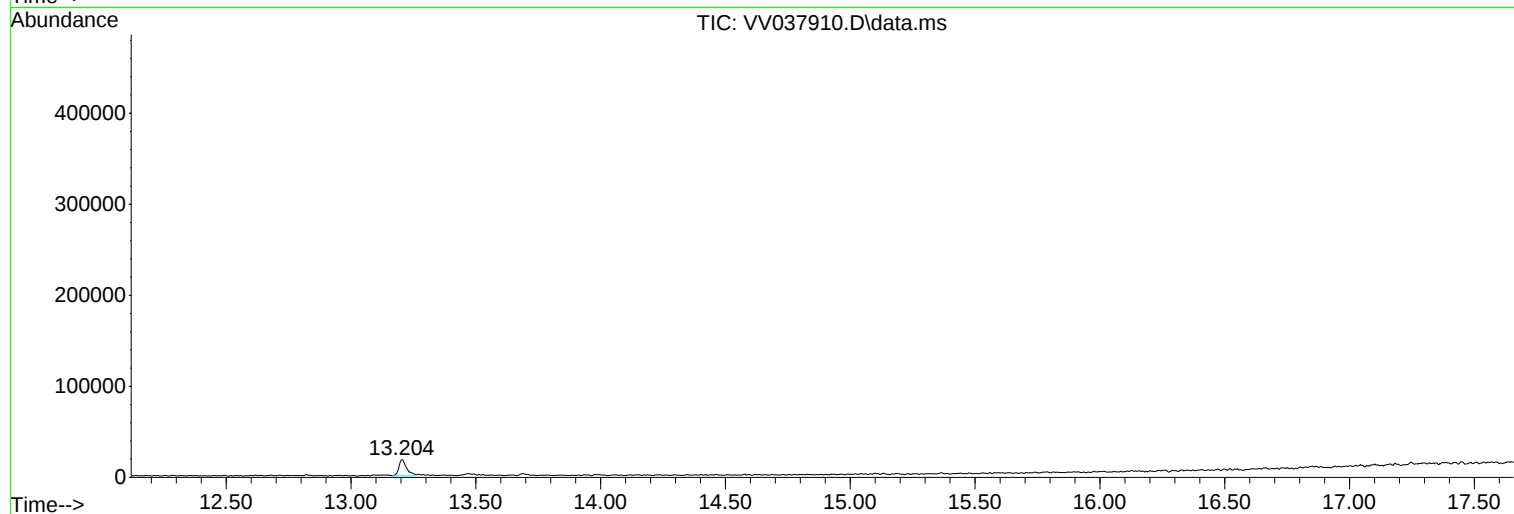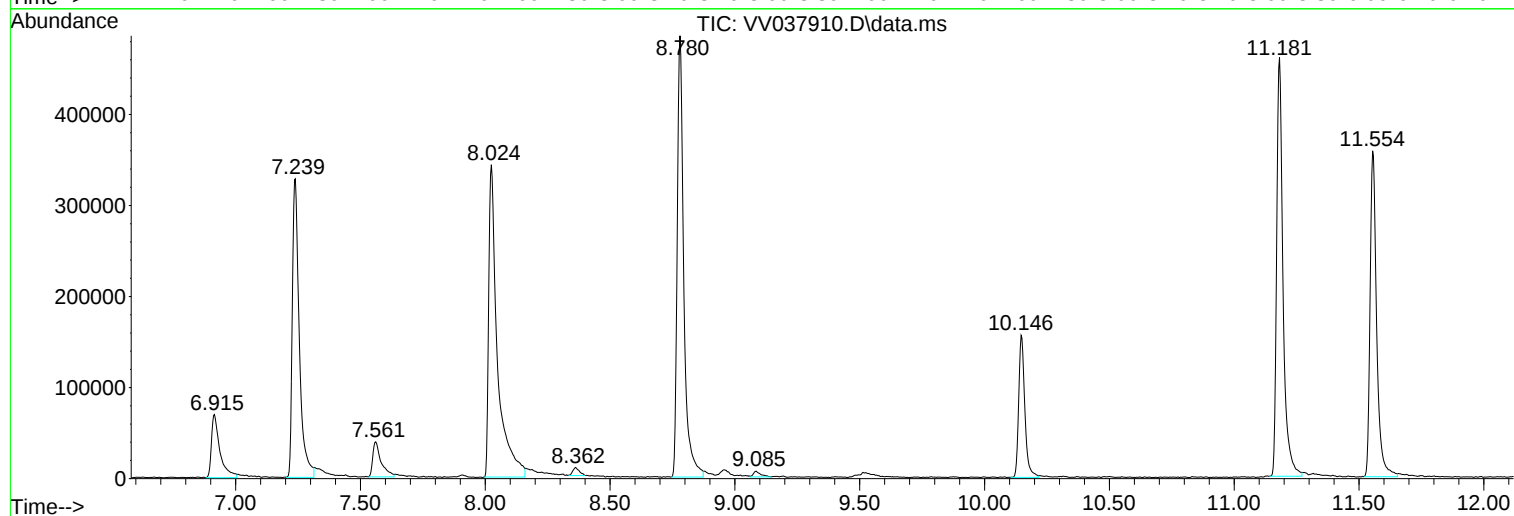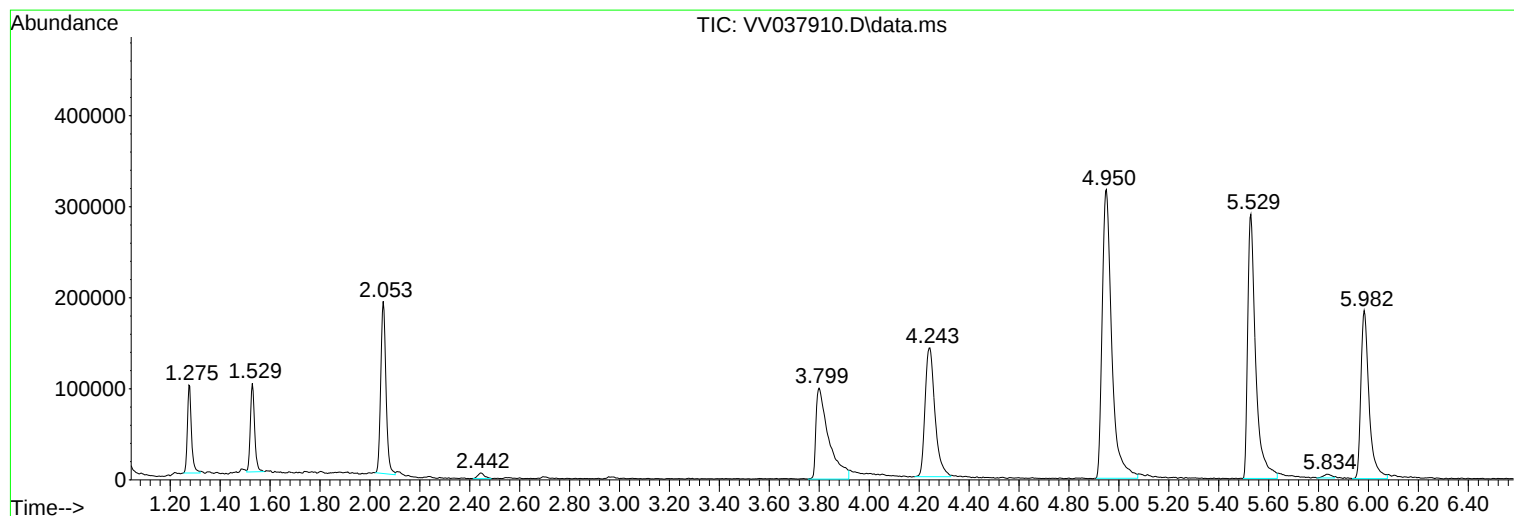

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102224\
Data File : VV037910.D
Acq On : 22 Oct 2024 14:41
Operator : SY/MD
Sample : VIBLK390
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK390

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102224\
Data File : VV037910.D
Acq On : 22 Oct 2024 14:41
Operator : SY/MD
Sample : VIBLK390
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK390

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc