
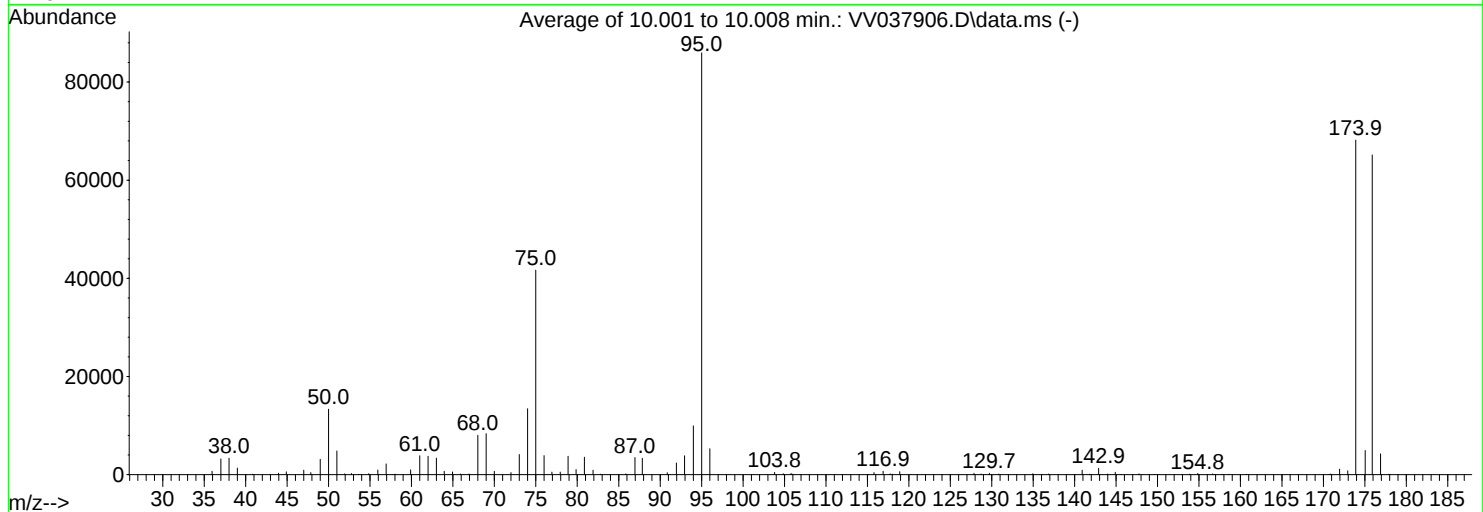


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102224\
Data File : VV037906.D
Acq On : 22 Oct 2024 08:15
Operator : SY/MD
Sample : BFB280
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB280

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Oct 23 01:16:33 2024

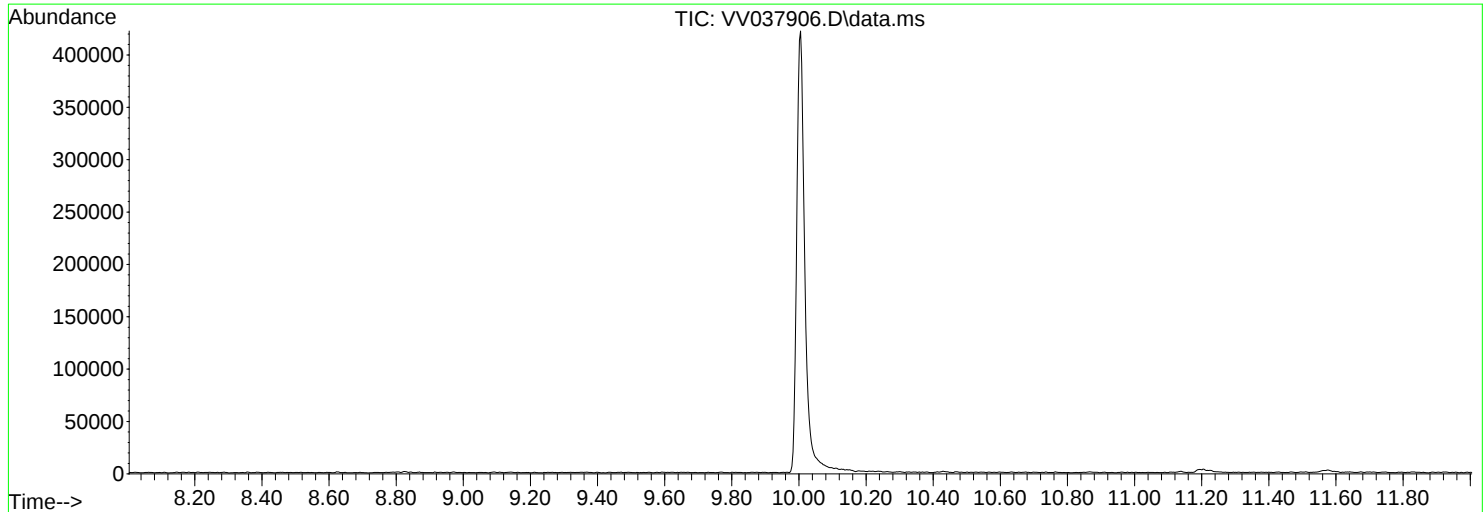

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	13342	PASS
75	95	30	80	48.5	41685	PASS
95	95	100	100	100.0	85952	PASS
96	95	5	9	6.1	5283	PASS
173	174	0.00	2	1.2	794	PASS
174	95	50	120	79.3	68165	PASS
175	174	5	9	7.2	4919	PASS
176	174	95	105	95.6	65133	PASS
177	176	5	10	6.5	4246	PASS

m/z	Abundance
39.90	598.0
43.10	138.0
43.90	640.0
44.80	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB280

m/z	Abundance
35.90	613.0
37.00	3424.0
38.00	3552.0
39.00	1406.0
39.80	554.0
44.00	983.0
45.00	727.0
46.00	132.0
47.00	862.0
47.90	476.0
49.00	3193.0
50.00	13706.0
51.00	4955.0
52.00	203.0
52.70	225.0
53.70	110.0
54.90	214.0
55.90	985.0
57.00	2176.0
57.80	134.0
59.90	951.0
61.00	4024.0
62.00	3656.0
63.00	3356.0
63.90	679.0
64.90	528.0
65.90	154.0
66.90	212.0
68.00	8212.0
69.00	8448.0
70.00	709.0
72.00	404.0
73.00	4417.0
74.00	13689.0
75.00	42688.0
76.00	3964.0
77.00	572.0
77.90	479.0
78.90	3790.0
79.90	1133.0
80.90	3534.0
81.90	756.0
85.90	190.0
87.00	3481.0
87.80	3070.0
90.90	376.0
92.00	2483.0
92.90	3717.0
94.00	9909.0
95.00	88040.0
96.00	5367.0
103.80	451.0
104.90	214.0
105.80	390.0
115.70	391.0
116.90	679.0
117.70	258.0
118.90	677.0
127.80	284.0
128.60	116.0
129.70	283.0
130.80	132.0
135.00	200.0
136.90	159.0
140.90	978.0
142.90	1467.0
143.90	162.0
144.90	511.0
145.60	122.0
147.70	139.0
153.90	105.0
154.80	245.0
156.70	202.0
160.70	101.0
170.70	208.0
171.90	989.0
173.00	765.0
173.90	67672.0
175.00	5010.0
175.90	64992.0
176.90	4392.0

Instrument :
MSVOA_V
ClientSampleId :
BFB280

m/z	Abundance
35.90	747.0
37.00	3175.0
38.00	3460.0
39.00	1383.0
39.80	503.0
40.80	150.0
44.00	930.0
44.90	732.0
47.00	969.0
47.90	410.0
49.00	3234.0
50.00	13726.0
51.00	4952.0
51.90	154.0
52.70	271.0
54.90	195.0
55.90	981.0
56.90	2250.0
58.00	119.0
59.90	1009.0
61.00	3997.0
62.00	3866.0
63.00	3446.0
63.90	693.0
64.90	546.0
65.90	158.0
67.00	141.0
68.00	8195.0
69.00	8673.0
70.00	731.0
72.00	440.0
73.00	4170.0
74.00	13678.0
75.00	43256.0
76.00	4067.0
77.00	493.0
78.00	565.0
78.90	3901.0
79.90	1060.0
80.90	3687.0
81.90	973.0
82.80	121.0
85.90	193.0
87.00	3593.0
87.80	3453.0
90.90	405.0
91.90	2385.0
93.00	3954.0
94.00	10250.0
95.00	88848.0
96.00	5424.0
103.80	514.0
104.90	188.0
105.80	359.0
115.80	438.0
116.90	711.0
118.00	268.0
118.90	634.0
127.90	302.0
128.70	143.0
129.70	313.0
130.90	133.0
135.00	226.0
136.80	140.0
140.90	914.0
141.80	131.0
142.90	1357.0
143.90	140.0
144.90	500.0
147.70	155.0
153.90	120.0
154.90	268.0
156.60	191.0
157.80	103.0
158.60	119.0
160.70	101.0
170.90	191.0
171.90	1159.0
172.90	791.0
173.90	70592.0
175.00	5177.0
175.90	67280.0
176.90	4406.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB280

m/z	Abundance
36.00	746.0
37.00	3029.0
38.00	3024.0
39.00	1270.0
39.90	506.0
40.90	194.0
44.00	917.0
45.00	591.0
47.00	927.0
47.80	374.0
49.00	2978.0
50.00	12594.0
51.00	4545.0
51.90	151.0
52.80	209.0
53.60	127.0
54.80	169.0
56.00	858.0
56.90	2121.0
58.10	138.0
59.90	931.0
61.00	3580.0
62.00	3687.0
63.00	3264.0
64.00	734.0
65.00	548.0
65.90	104.0
68.00	7645.0
69.00	7941.0
70.00	610.0
72.00	469.0
73.00	3729.0
74.00	12907.0
75.00	39112.0
76.00	3594.0
76.90	467.0
78.00	574.0
78.90	3595.0
79.80	968.0
80.80	3481.0
81.90	993.0
82.80	145.0
85.80	151.0
86.90	3436.0
87.90	3463.0
90.80	374.0
91.90	2259.0
93.00	3853.0
94.00	9695.0
95.00	80968.0
96.00	5058.0
103.80	423.0
104.80	154.0
106.00	318.0
106.90	115.0
115.10	129.0
115.90	433.0
116.90	654.0
117.80	257.0
118.90	574.0
127.90	272.0
128.80	174.0
129.70	286.0
130.90	138.0
134.90	216.0
136.80	131.0
140.90	840.0
141.80	146.0
142.90	1144.0
144.00	124.0
144.90	492.0
147.80	159.0
149.00	120.0
149.60	112.0
153.90	107.0
154.90	252.0
156.60	150.0
156.90	141.0
157.80	105.0
158.60	114.0
170.90	168.0
172.00	1181.0
172.90	826.0
173.90	66232.0
175.10	4570.0
175.90	63128.0
176.90	3939.0
177.90	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB280