

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
 Data File : VV037914.D
 Acq On : 23 Oct 2024 11:21
 Operator : SY/MD
 Sample : VV1023MBL01
 Misc : 5.00g/5mL/100ul/5mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK253

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rVB	252395	264441	12.24%	1.770%
2	1.532	146	153	168	rVB	228165	272916	12.63%	1.827%
3	2.060	308	317	330	rVB	480015	683486	31.63%	4.576%
4	3.500	760	765	768	rBV	903	706	0.03%	0.005%
5	3.529	772	774	776	rBV2	445	225	0.01%	0.002%
6	3.616	799	801	802	rBV	399	160	0.01%	0.001%
7	3.683	820	822	824	rBV3	497	300	0.01%	0.002%
8	3.728	834	836	837	rBV2	413	162	0.01%	0.001%
9	3.764	845	847	849	rBV	680	285	0.01%	0.002%
10	3.799	849	858	902	rBV	100666	312619	14.47%	2.093%
11	4.134	959	962	967	rBV4	1181	1214	0.06%	0.008%
12	4.243	980	996	1025	rBV	355296	913990	42.30%	6.119%
13	4.506	1073	1078	1080	rBV4	1402	1188	0.05%	0.008%
14	4.561	1093	1095	1099	rVB3	714	409	0.02%	0.003%
15	4.590	1102	1104	1107	rVB4	640	276	0.01%	0.002%
16	4.632	1115	1117	1123	rVB4	796	499	0.02%	0.003%
17	4.667	1126	1128	1130	rBV3	312	152	0.01%	0.001%
18	4.703	1136	1139	1143	rVB4	655	505	0.02%	0.003%
19	4.725	1143	1146	1149	rBV2	772	475	0.02%	0.003%
20	4.796	1165	1168	1170	rVB	706	414	0.02%	0.003%
21	4.809	1170	1172	1174	rBV2	378	191	0.01%	0.001%
22	4.822	1174	1176	1178	rVB2	284	108	0.00%	0.001%
23	4.844	1178	1183	1186	rBV5	824	942	0.04%	0.006%
24	4.892	1196	1198	1199	rBV	385	171	0.01%	0.001%
25	4.950	1199	1216	1250	rBV2	849560	2160871	100.00%	14.466%
26	5.432	1364	1366	1368	rBV2	469	168	0.01%	0.001%
27	5.529	1385	1396	1425	rBV	502060	1050481	48.61%	7.032%
28	5.831	1479	1490	1505	rBV8	11935	30943	1.43%	0.207%
29	5.982	1525	1537	1571	rBV	478603	1002242	46.38%	6.709%
30	6.310	1637	1639	1641	rBV2	538	207	0.01%	0.001%
31	6.330	1641	1645	1648	rBV3	574	481	0.02%	0.003%
32	6.371	1656	1658	1660	rBV	244	102	0.00%	0.001%
33	6.381	1660	1661	1664	rVB	253	89	0.00%	0.001%
34	6.400	1664	1667	1670	rBV3	637	500	0.02%	0.003%
35	6.497	1693	1697	1700	rBV2	538	405	0.02%	0.003%
36	6.522	1703	1705	1709	rVB	301	175	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
 Data File : VV037914.D
 Acq On : 23 Oct 2024 11:21
 Operator : SY/MD
 Sample : VV1023MBL01
 Misc : 5.00g/5mL/100ul/5mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK253

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.548	1709	1713	1721	rBV6	1032	1064	0.05%	0.007%
38	6.587	1721	1725	1729	rBV3	387	349	0.02%	0.002%
39	6.654	1743	1746	1749	rBV3	1014	674	0.03%	0.005%
40	6.712	1760	1764	1765	rBV3	676	368	0.02%	0.002%
41	6.725	1765	1768	1773	rBV4	967	886	0.04%	0.006%
42	6.786	1785	1787	1792	rVB3	824	542	0.03%	0.004%
43	6.809	1792	1794	1795	rBV	164	82	0.00%	0.001%
44	6.825	1795	1799	1801	rVB2	668	424	0.02%	0.003%
45	6.850	1803	1807	1808	rBV2	272	147	0.01%	0.001%
46	6.908	1812	1825	1851	rBV	227246	442097	20.46%	2.960%
47	7.236	1917	1927	1957	rBV	921020	1647073	76.22%	11.026%
48	7.551	2016	2025	2053	rBV	151660	290245	13.43%	1.943%
49	7.866	2118	2123	2128	rBV5	1202	1553	0.07%	0.010%
50	8.024	2164	2172	2216	rBV2	292819	660341	30.56%	4.421%
51	8.780	2393	2407	2439	rBV	807422	1372197	63.50%	9.186%
52	9.217	2541	2543	2545	rBV2	694	437	0.02%	0.003%
53	9.249	2551	2553	2557	rBV5	403	297	0.01%	0.002%
54	9.281	2560	2563	2564	rBV	401	209	0.01%	0.001%
55	9.333	2577	2579	2582	rBV2	477	311	0.01%	0.002%
56	9.413	2599	2604	2605	rBV3	606	484	0.02%	0.003%
57	9.436	2609	2611	2615	rVB2	737	378	0.02%	0.003%
58	9.464	2618	2620	2623	rBV	603	318	0.01%	0.002%
59	9.487	2623	2627	2628	rBV2	1012	835	0.04%	0.006%
60	9.567	2650	2652	2653	rBV	339	100	0.00%	0.001%
61	9.667	2680	2683	2686	rBV2	556	471	0.02%	0.003%
62	9.712	2693	2697	2699	rBV2	600	405	0.02%	0.003%
63	9.725	2699	2701	2705	rVV4	424	292	0.01%	0.002%
64	9.786	2716	2720	2724	rBV3	422	433	0.02%	0.003%
65	9.844	2735	2738	2741	rBV3	461	367	0.02%	0.002%
66	9.931	2763	2765	2770	rVB3	676	571	0.03%	0.004%
67	9.956	2770	2773	2775	rBV2	242	186	0.01%	0.001%
68	9.985	2779	2782	2783	rBV2	594	263	0.01%	0.002%
69	10.053	2799	2803	2805	rBV3	651	546	0.03%	0.004%
70	10.146	2819	2832	2863	rBV	592737	952302	44.07%	6.375%
71	10.455	2926	2928	2930	rBV3	544	277	0.01%	0.002%
72	10.513	2942	2946	2949	rBV2	693	651	0.03%	0.004%
73	10.744	3016	3018	3021	rVB	480	226	0.01%	0.002%
74	10.776	3021	3028	3029	rBV3	1071	819	0.04%	0.005%
75	10.802	3034	3036	3039	rVV3	642	367	0.02%	0.002%
76	10.857	3047	3053	3056	rBV5	1736	2169	0.10%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
 Data File : VV037914.D
 Acq On : 23 Oct 2024 11:21
 Operator : SY/MD
 Sample : VV1023MBL01
 Misc : 5.00g/5mL/100ul/5ml/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK253

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

77	10.927	3074	3075	3076	rBV5	201	49	0.00%	0.000%
78	10.934	3076	3077	3079	rBV	453	153	0.01%	0.001%
79	11.053	3109	3114	3115	rBV2	1005	692	0.03%	0.005%
80	11.127	3127	3137	3143	rBV6	3251	5727	0.27%	0.038%
81	11.178	3143	3153	3191	rVV	786802	1272626	58.89%	8.520%
82	11.464	3237	3242	3246	rBV4	1219	1261	0.06%	0.008%
83	11.551	3258	3269	3303	rBV	951348	1544009	71.45%	10.336%
84	11.972	3397	3400	3402	rBV2	760	439	0.02%	0.003%
85	12.111	3441	3443	3444	rBV	406	147	0.01%	0.001%
86	12.133	3448	3450	3452	rBV2	637	342	0.02%	0.002%
87	12.371	3521	3524	3526	rBV	1079	745	0.03%	0.005%
88	12.445	3545	3547	3551	rVB3	842	386	0.02%	0.003%
89	13.210	3778	3785	3798	rBV9	5316	9282	0.43%	0.062%
90	13.448	3852	3859	3871	rBV3	9705	17642	0.82%	0.118%




Sum of corrected areas: 14937754

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
Data File : VV037914.D
Acq On : 23 Oct 2024 11:21
Operator : SY/MD
Sample : VV1023MBL01
Misc : 5.00g/5mL/100ul/5mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

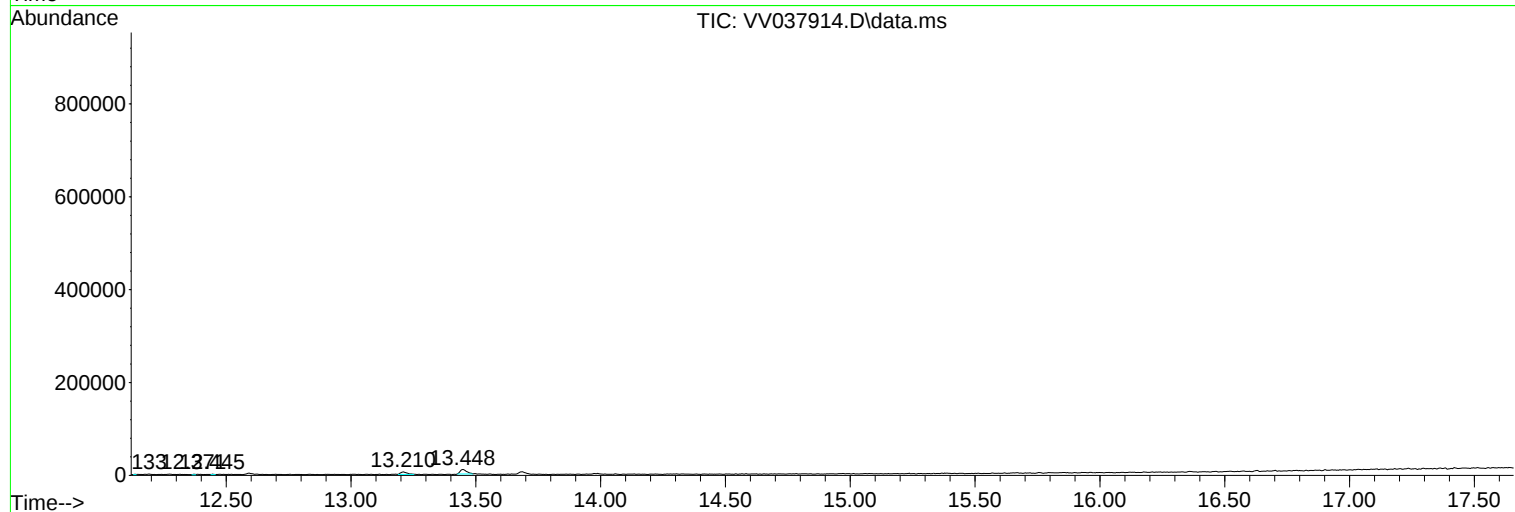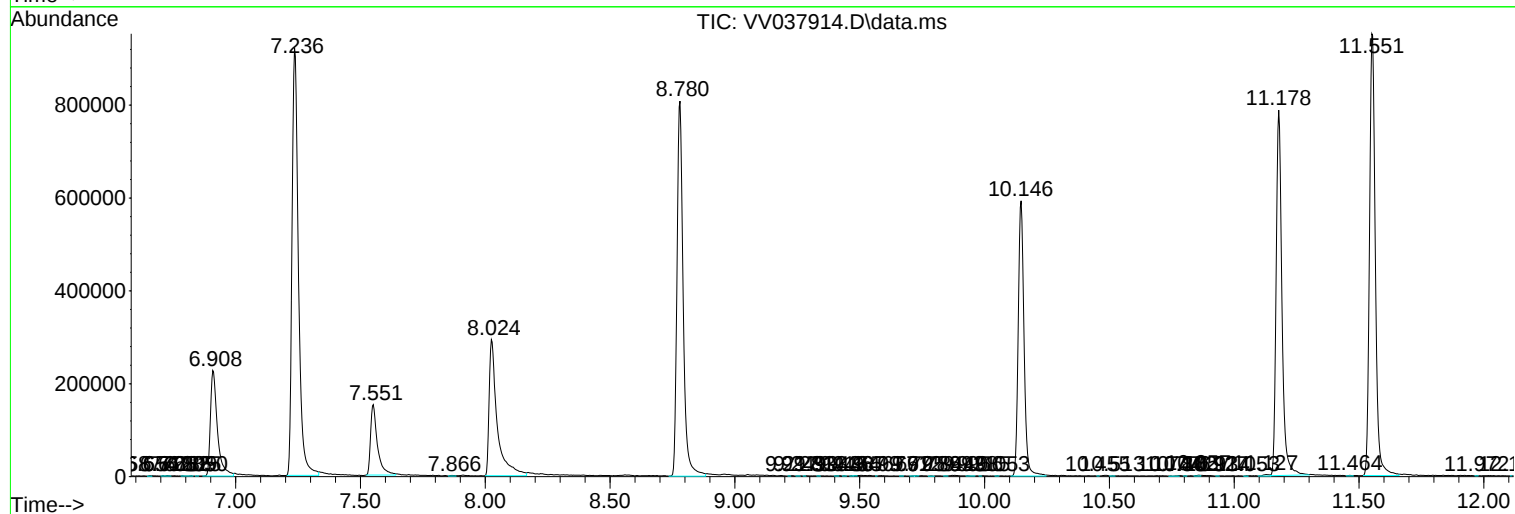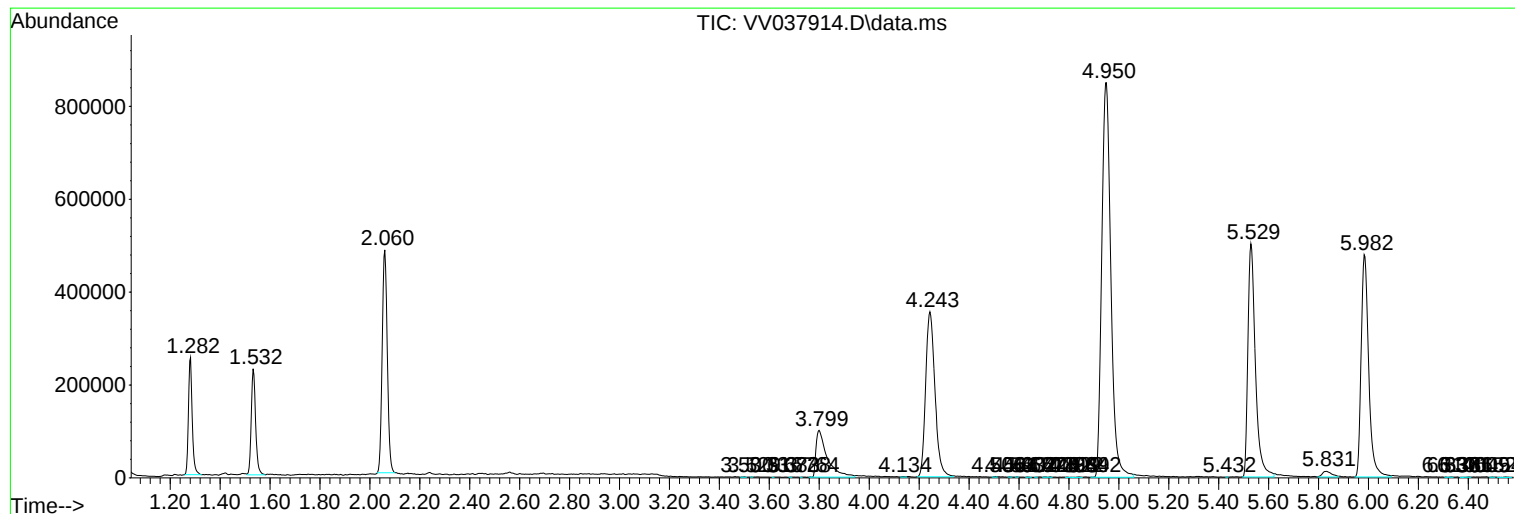

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
Data File : VV037914.D
Acq On : 23 Oct 2024 11:21
Operator : SY/MD
Sample : VV1023MBL01
Misc : 5.00g/5mL/100ul/5ml/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
Data File : VV037914.D
Acq On : 23 Oct 2024 11:21
Operator : SY/MD
Sample : VV1023MBL01
Misc : 5.00g/5mL/100ul/5ml/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc