

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
 Data File : VV037917.D
 Acq On : 23 Oct 2024 15:16
 Operator : SY/MD
 Sample : P4436-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	44	rBV2	8059	8291	0.43%	0.054%
2	1.217	52	55	63	rVB2	3208	3092	0.16%	0.020%
3	1.278	68	74	87	rVB	226286	235413	12.10%	1.543%
4	1.532	145	153	170	rVB	209845	250797	12.89%	1.644%
5	2.056	307	316	327	rBV	420726	598584	30.76%	3.924%
6	2.114	328	334	350	rVB	33437	52107	2.68%	0.342%
7	3.336	710	714	716	rBV4	749	710	0.04%	0.005%
8	3.632	802	806	809	rVB3	764	600	0.03%	0.004%
9	3.796	848	857	885	rBV	98230	280089	14.39%	1.836%
10	4.114	953	956	959	rVB2	1115	735	0.04%	0.005%
11	4.130	959	961	970	rBB4	867	943	0.05%	0.006%
12	4.236	977	994	1022	rBV	331615	845686	43.46%	5.543%
13	4.394	1041	1043	1049	rVB4	949	849	0.04%	0.006%
14	4.548	1087	1091	1094	rBV4	939	701	0.04%	0.005%
15	4.686	1128	1134	1136	rBV3	855	620	0.03%	0.004%
16	4.728	1141	1147	1149	rBV4	659	680	0.03%	0.004%
17	4.815	1168	1174	1175	rBV2	720	571	0.03%	0.004%
18	4.944	1199	1214	1251	rBV2	769645	1946065	100.00%	12.757%
19	5.133	1271	1273	1279	rVB5	1327	1067	0.05%	0.007%
20	5.201	1292	1294	1299	rVB5	891	669	0.03%	0.004%
21	5.339	1332	1337	1339	rBV5	786	589	0.03%	0.004%
22	5.403	1354	1357	1360	rVB2	913	551	0.03%	0.004%
23	5.465	1370	1376	1379	rBV3	717	698	0.04%	0.005%
24	5.526	1383	1395	1431	rBV	697224	1470068	75.54%	9.636%
25	5.825	1477	1488	1508	rVB4	14320	35682	1.83%	0.234%
26	5.902	1508	1512	1519	rVB5	1252	1184	0.06%	0.008%
27	5.979	1523	1536	1570	rBV	434581	921052	47.33%	6.038%
28	6.211	1606	1608	1611	rBV3	964	703	0.04%	0.005%
29	6.284	1626	1631	1634	rVB4	840	642	0.03%	0.004%
30	6.304	1634	1637	1639	rBV3	786	545	0.03%	0.004%
31	6.452	1677	1683	1684	rBV4	799	685	0.04%	0.004%
32	6.493	1693	1696	1701	rVB4	574	616	0.03%	0.004%
33	6.567	1716	1719	1724	rVB5	1159	1030	0.05%	0.007%
34	6.603	1726	1730	1735	rBV3	638	623	0.03%	0.004%
35	6.715	1761	1765	1770	rBV4	969	1189	0.06%	0.008%
36	6.747	1773	1775	1781	rVB2	909	842	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
 Data File : VV037917.D
 Acq On : 23 Oct 2024 15:16
 Operator : SY/MD
 Sample : P4436-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.799	1788	1791	1798	rVB7	696	656	0.03%	0.004%
38	6.908	1814	1825	1853	rBV	203913	405799	20.85%	2.660%
39	7.233	1915	1926	1961	rBV	792863	1438994	73.94%	9.433%
40	7.548	2015	2024	2048	rBV	132952	261756	13.45%	1.716%
41	7.876	2123	2126	2130	rBV4	708	581	0.03%	0.004%
42	8.024	2163	2172	2213	rBV2	272235	629251	32.33%	4.125%
43	8.326	2264	2266	2272	rVB4	1139	751	0.04%	0.005%
44	8.407	2288	2291	2295	rVB5	1326	1048	0.05%	0.007%
45	8.442	2297	2302	2306	rBV4	1063	909	0.05%	0.006%
46	8.545	2327	2334	2345	rVB8	1931	3787	0.19%	0.025%
47	8.590	2345	2348	2350	rBV2	794	614	0.03%	0.004%
48	8.641	2357	2364	2370	rBV7	1627	2537	0.13%	0.017%
49	8.776	2395	2406	2440	rBV	1102906	1834302	94.26%	12.024%
50	9.181	2529	2532	2539	rVB6	963	1063	0.05%	0.007%
51	9.506	2631	2633	2637	rVB4	959	590	0.03%	0.004%
52	9.567	2648	2652	2655	rBV3	713	564	0.03%	0.004%
53	9.612	2662	2666	2670	rVB3	723	563	0.03%	0.004%
54	9.718	2692	2699	2701	rBV4	1528	1570	0.08%	0.010%
55	9.831	2729	2734	2737	rBV4	846	741	0.04%	0.005%
56	9.886	2743	2751	2753	rBV5	2974	3822	0.20%	0.025%
57	9.947	2767	2770	2775	rBV4	636	663	0.03%	0.004%
58	10.146	2818	2832	2851	rBV	556700	888680	45.67%	5.825%
59	10.342	2889	2893	2896	rBV4	871	603	0.03%	0.004%
60	10.480	2933	2936	2943	rVB2	877	753	0.04%	0.005%
61	10.522	2943	2949	2950	rBV4	737	588	0.03%	0.004%
62	10.564	2957	2962	2963	rBV4	1293	915	0.05%	0.006%
63	10.638	2983	2985	2989	rVV4	946	593	0.03%	0.004%
64	10.776	3022	3028	3033	rBV5	915	1018	0.05%	0.007%
65	10.802	3033	3036	3039	rBV2	936	809	0.04%	0.005%
66	11.123	3127	3136	3142	rVV7	5529	9215	0.47%	0.060%
67	11.178	3142	3153	3187	rVV	1008451	1630826	83.80%	10.690%
68	11.458	3237	3240	3245	rBV6	1020	883	0.05%	0.006%
69	11.506	3250	3255	3256	rBV3	3297	2740	0.14%	0.018%
70	11.551	3258	3269	3297	rVV	881195	1434730	73.72%	9.405%
71	11.783	3338	3341	3346	rVB6	1504	1450	0.07%	0.010%
72	11.815	3346	3351	3353	rBV4	929	920	0.05%	0.006%
73	11.834	3353	3357	3362	rBV5	2508	2325	0.12%	0.015%
74	12.220	3474	3477	3481	rBV5	1039	1026	0.05%	0.007%
75	12.297	3498	3501	3502	rBV2	1562	970	0.05%	0.006%
76	12.615	3596	3600	3604	rVB5	622	617	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
 Data File : VV037917.D
 Acq On : 23 Oct 2024 15:16
 Operator : SY/MD
 Sample : P4436-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.670	3613	3617	3619	rBV3	1042	676	0.03%	0.004%
78	12.712	3628	3630	3635	rVB4	998	599	0.03%	0.004%
79	12.795	3651	3656	3660	rVB3	972	834	0.04%	0.005%
80	12.895	3685	3687	3691	rBV6	912	677	0.03%	0.004%
81	12.940	3699	3701	3706	rBV4	995	747	0.04%	0.005%
82	13.162	3767	3770	3775	rBV3	942	776	0.04%	0.005%
83	13.213	3782	3786	3791	rBV7	1370	1063	0.05%	0.007%
84	13.242	3792	3795	3797	rBV3	904	568	0.03%	0.004%
85	13.281	3805	3807	3811	rVB3	821	618	0.03%	0.004%
86	13.307	3811	3815	3819	rBV5	759	841	0.04%	0.006%
87	13.416	3847	3849	3853	rVB4	735	514	0.03%	0.003%
88	13.448	3856	3859	3861	rBV3	1042	671	0.03%	0.004%
89	13.464	3861	3864	3868	rBV5	1498	1128	0.06%	0.007%
90	13.525	3880	3883	3890	rVB5	1281	1045	0.05%	0.007%
91	13.689	3930	3934	3937	rBV6	1131	1019	0.05%	0.007%
92	13.728	3943	3946	3950	rBV5	1019	899	0.05%	0.006%
93	13.815	3968	3973	3979	rBV6	1143	1494	0.08%	0.010%
94	14.040	4040	4043	4047	rBV4	792	650	0.03%	0.004%
95	14.156	4077	4079	4086	rBV4	1122	1224	0.06%	0.008%
96	14.458	4171	4173	4176	rBV2	818	509	0.03%	0.003%
97	14.615	4220	4222	4226	rBV3	584	526	0.03%	0.003%
98	15.020	4346	4348	4350	rBV2	1075	559	0.03%	0.004%
99	15.056	4355	4359	4364	rVV8	1718	1913	0.10%	0.013%
100	15.139	4382	4385	4386	rBV3	1359	731	0.04%	0.005%




Sum of corrected areas: 15255471

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
Data File : VV037917.D
Acq On : 23 Oct 2024 15:16
Operator : SY/MD
Sample : P4436-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

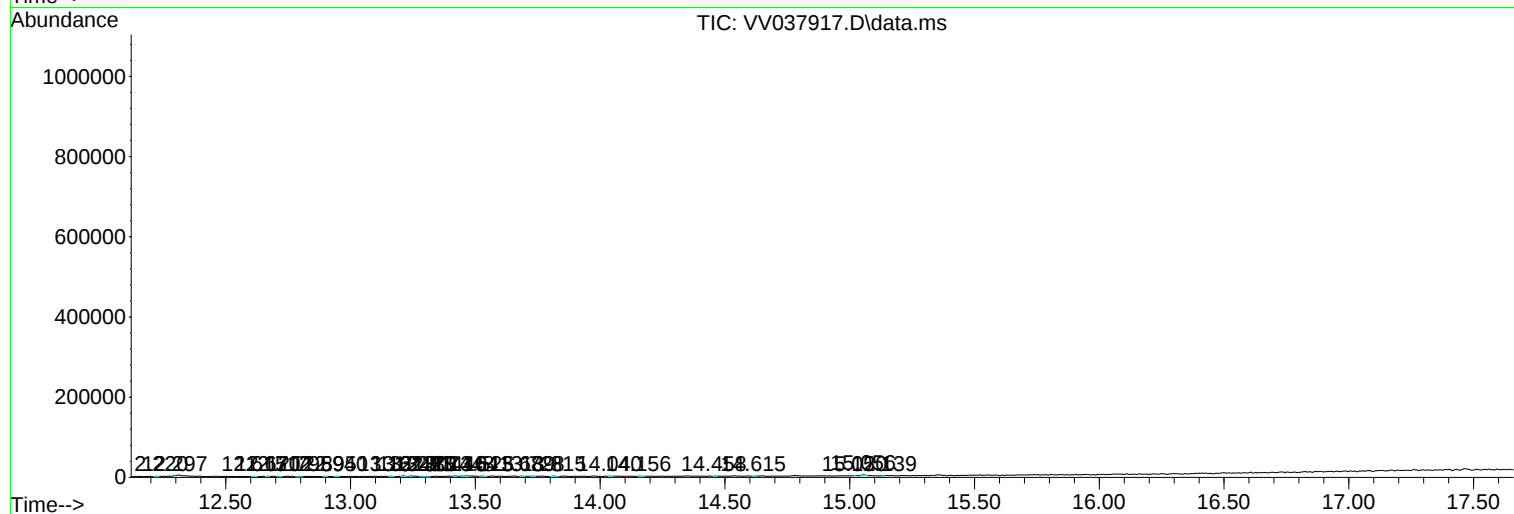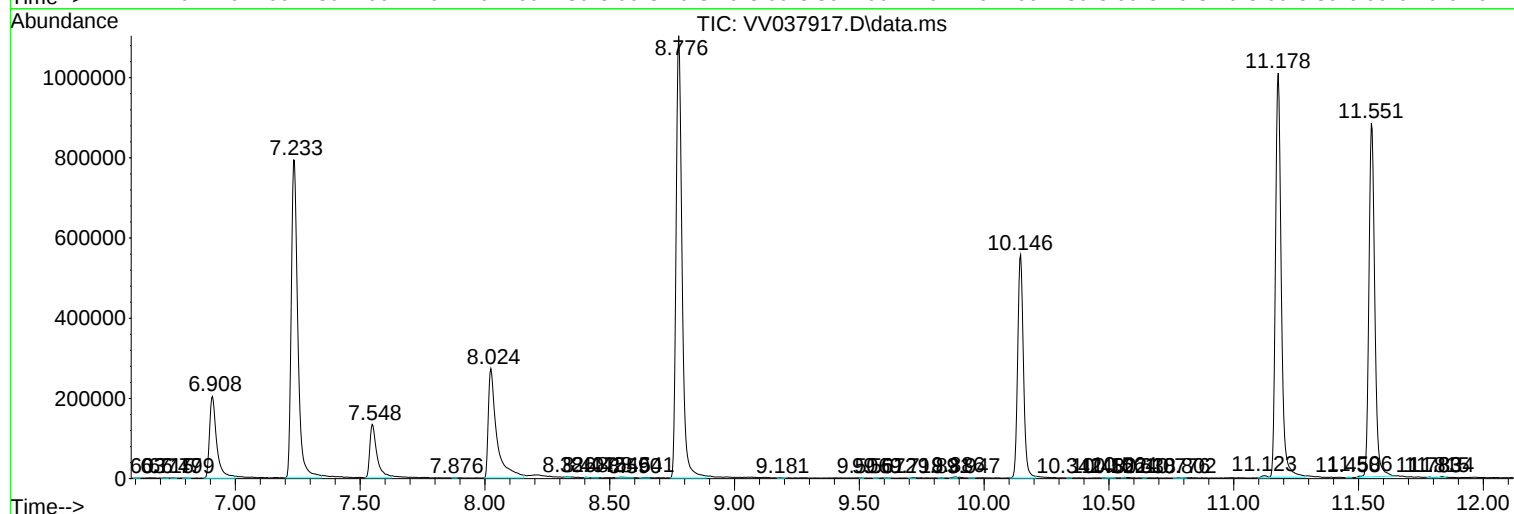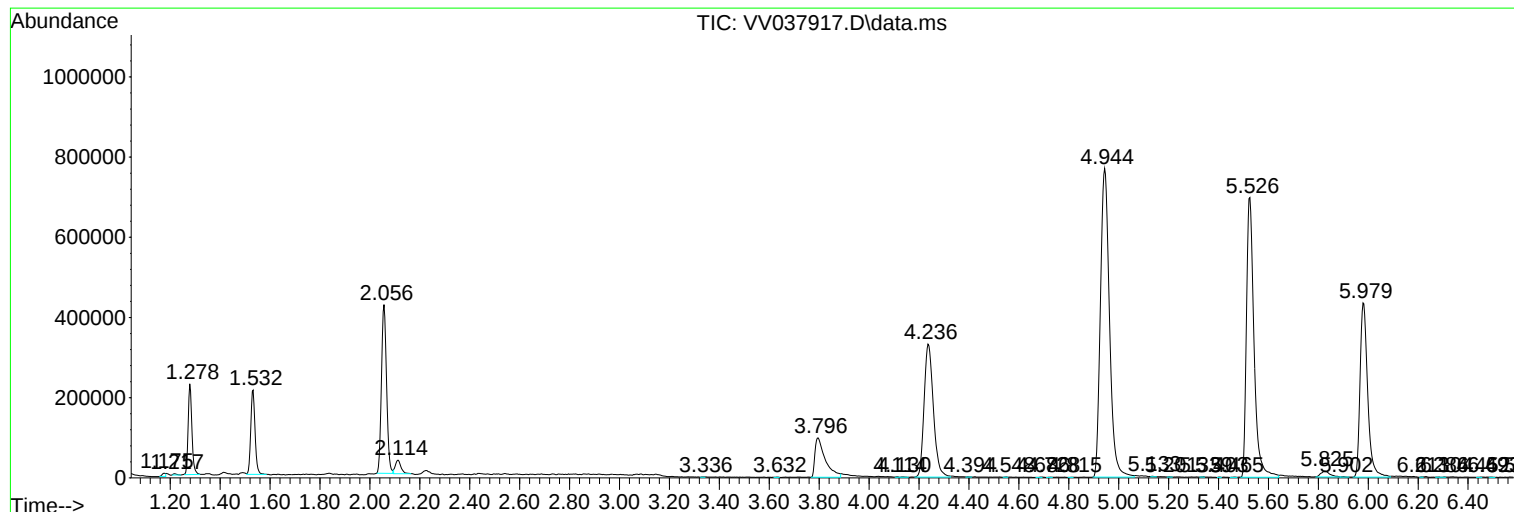

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
Data File : VV037917.D
Acq On : 23 Oct 2024 15:16
Operator : SY/MD
Sample : P4436-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
Data File : VV037917.D
Acq On : 23 Oct 2024 15:16
Operator : SY/MD
Sample : P4436-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------