
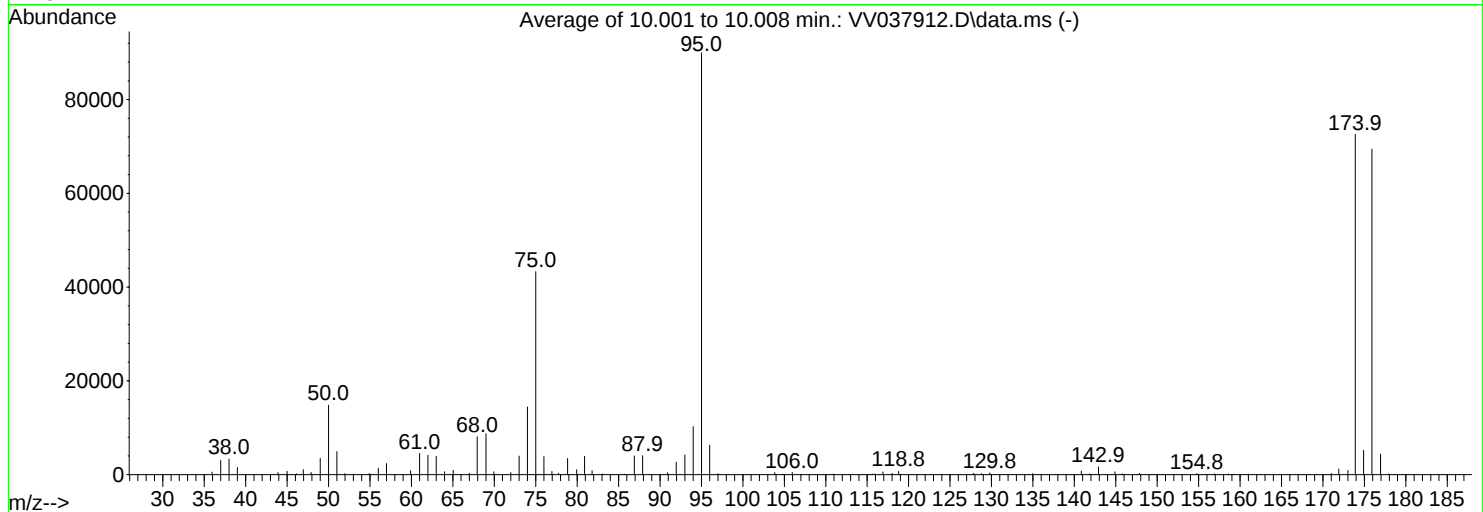


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV102324\
Data File : VV037912.D
Acq On : 23 Oct 2024 08:15
Operator : SY/MD
Sample : BFB398
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB398

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Tue Oct 22 05:07:16 2024

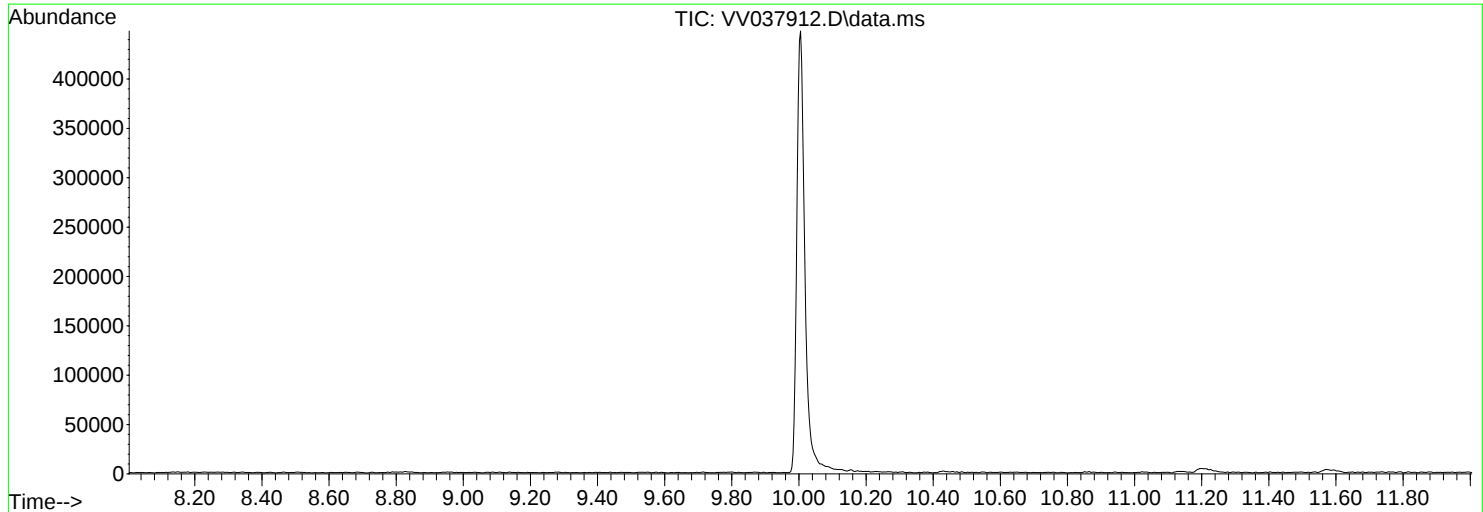

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	14828	PASS
75	95	30	80	48.1	43299	PASS
95	95	100	100	100.0	89963	PASS
96	95	5	9	7.0	6293	PASS
173	174	0.00	2	1.2	872	PASS
174	95	50	120	80.7	72584	PASS
175	174	5	9	7.2	5192	PASS
176	174	95	105	95.7	69440	PASS
177	176	5	10	6.3	4381	PASS

m/z	Abundance
39.90	667.0
43.80	645.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398

m/z	Abundance
35.90	582.0
37.00	3136.0
38.00	3352.0
39.00	1508.0
39.90	676.0
43.10	104.0
44.00	972.0
45.00	763.0
46.20	149.0
46.90	1064.0
47.80	478.0
49.00	3445.0
50.00	15060.0
51.00	5302.0
51.90	184.0
53.10	149.0
54.00	109.0
54.90	333.0
56.00	1375.0
57.00	2628.0
59.90	912.0
61.00	4647.0
62.00	4214.0
63.00	3692.0
64.00	585.0
65.10	931.0
66.00	110.0
67.00	338.0
67.90	8358.0
69.00	8919.0
69.90	591.0
72.00	487.0
73.00	4150.0
74.00	15076.0
75.00	43912.0
76.00	3874.0
77.00	728.0
77.80	299.0
78.90	3475.0
79.90	1109.0
80.90	3957.0
81.80	849.0
83.10	174.0
86.90	4383.0
87.90	4178.0
90.90	402.0
92.00	2662.0
93.00	4360.0
94.00	10697.0
95.00	91400.0
96.00	6555.0
97.00	269.0
103.90	432.0
104.80	194.0
105.90	486.0
107.00	148.0
110.90	148.0
115.60	226.0
116.00	201.0
116.80	568.0
118.00	318.0
118.80	735.0
127.80	313.0
128.80	184.0
129.80	384.0
135.00	251.0
139.90	133.0
140.80	795.0
141.80	202.0
142.90	1650.0
144.90	585.0
145.80	191.0
147.80	249.0
149.90	116.0
154.80	244.0
156.90	185.0
158.60	127.0
171.00	235.0
171.90	1053.0
173.00	789.0
173.90	71368.0
174.90	5407.0
175.90	67968.0
176.90	4611.0
178.00	239.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398

m/z	Abundance
36.00	559.0
37.00	3089.0
38.00	3449.0
39.00	1546.0
39.90	583.0
44.00	1105.0
45.00	733.0
46.10	180.0
47.00	1178.0
47.90	496.0
49.00	3653.0
50.00	15299.0
51.00	4971.0
51.90	197.0
53.10	150.0
54.90	249.0
56.00	1408.0
57.00	2474.0
59.90	887.0
61.00	4730.0
62.00	4300.0
63.00	4066.0
64.00	642.0
65.10	967.0
65.90	105.0
67.00	328.0
68.00	8192.0
69.00	8935.0
70.00	646.0
72.00	462.0
73.00	4067.0
74.00	15085.0
75.00	44520.0
76.00	3932.0
77.00	704.0
77.80	308.0
78.80	3554.0
80.00	1082.0
80.90	4029.0
81.80	872.0
83.10	167.0
85.70	161.0
86.90	4071.0
87.90	4258.0
90.90	415.0
91.90	2690.0
93.00	4351.0
94.00	10541.0
95.00	93288.0
96.00	6558.0
97.00	211.0
103.90	446.0
104.80	136.0
106.00	491.0
107.10	119.0
110.90	146.0
112.80	106.0
115.60	186.0
116.00	162.0
116.90	570.0
118.00	285.0
118.80	736.0
127.90	323.0
128.80	193.0
129.80	386.0
135.00	224.0
140.80	772.0
141.80	185.0
142.90	1735.0
144.90	639.0
145.80	171.0
147.90	288.0
154.80	260.0
156.90	167.0
158.60	168.0
159.20	115.0
161.00	133.0
171.00	268.0
171.90	1229.0
173.00	891.0
173.90	74960.0
174.90	5304.0
175.90	71744.0
177.00	4514.0
177.90	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398

m/z	Abundance
36.00	524.0
37.00	2940.0
38.00	3190.0
39.00	1559.0
39.80	519.0
43.00	104.0
44.00	1215.0
45.00	657.0
46.10	171.0
47.00	1070.0
48.00	462.0
49.00	3308.0
50.00	14124.0
51.00	4509.0
52.00	253.0
53.00	140.0
54.90	173.0
55.10	170.0
56.00	1311.0
57.00	1960.0
59.90	789.0
61.00	4158.0
62.00	3920.0
63.00	3944.0
64.00	672.0
65.00	895.0
67.00	236.0
68.00	7691.0
69.00	8366.0
70.00	662.0
72.00	375.0
73.00	3617.0
74.00	13168.0
75.00	41464.0
76.00	3785.0
76.90	669.0
77.70	338.0
78.80	3310.0
80.00	964.0
80.90	3668.0
81.80	833.0
82.90	104.0
83.20	116.0
85.70	201.0
86.90	3530.0
87.90	3680.0
90.90	417.0
91.90	2516.0
93.00	3875.0
94.00	9482.0
95.00	85200.0
96.00	5765.0
97.00	143.0
103.80	417.0
105.10	138.0
106.00	429.0
110.90	124.0
112.80	106.0
115.90	171.0
117.00	579.0
118.00	270.0
118.80	607.0
127.90	269.0
128.80	213.0
129.80	343.0
134.80	193.0
140.90	671.0
141.90	148.0
142.90	1513.0
144.90	619.0
145.80	151.0
147.90	303.0
154.80	268.0
156.90	174.0
158.60	158.0
159.20	112.0
161.00	171.0
171.00	265.0
171.90	1267.0
173.00	936.0
173.90	71424.0
174.90	4866.0
175.90	68608.0
177.00	4017.0
177.90	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398