

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102523\
 Data File : VW032627.D
 Acq On : 25 Oct 2023 12:50
 Operator : SY/MD
 Sample : 04950-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 26 05:02:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 26 04:59:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	88689	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	101722	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	44777	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	35075	4.863	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	97.200%	
7) Chloroethane-d5	1.532	69	32741	5.592	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	111.800%	
11) 1,1-Dichloroethene-d2	2.056	65	14346	4.716	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	94.400%	
20) 2-Butanone-d5	3.825	46	66804	36.612	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	73.220%	
24) Chloroform-d	4.253	84	57303	4.503	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.000%	
26) 1,2-Dichloroethane-d4	4.947	65	30726	5.098	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.000%	
32) Benzene-d6	4.963	84	118435	3.957	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	79.200%	
36) 1,2-Dichloropropane-d6	5.992	67	37315	3.763	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	75.200%	
41) Toluene-d8	7.246	98	108979	3.982	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.600%	
43) trans-1,3-Dichloroprop...	7.561	79	13669	3.890	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	77.800%	
46) 2-Hexanone-d5	8.034	63	63696	38.524	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	77.040%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	31590	4.554	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.000%	
66) 1,2-Dichlorobenzene-d4	11.564	152	39889	4.801	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.000%	
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.921	75	1330	0.098	ug/L #	72
61) 1,2,3-Trichloropropane	11.188	75	5893	1.236	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032627.D
Acq On : 25 Oct 2023 12:50
Operator : SY/MD
Sample : 04950-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 26 05:02:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 26 04:59:52 2023
Response via : Initial Calibration

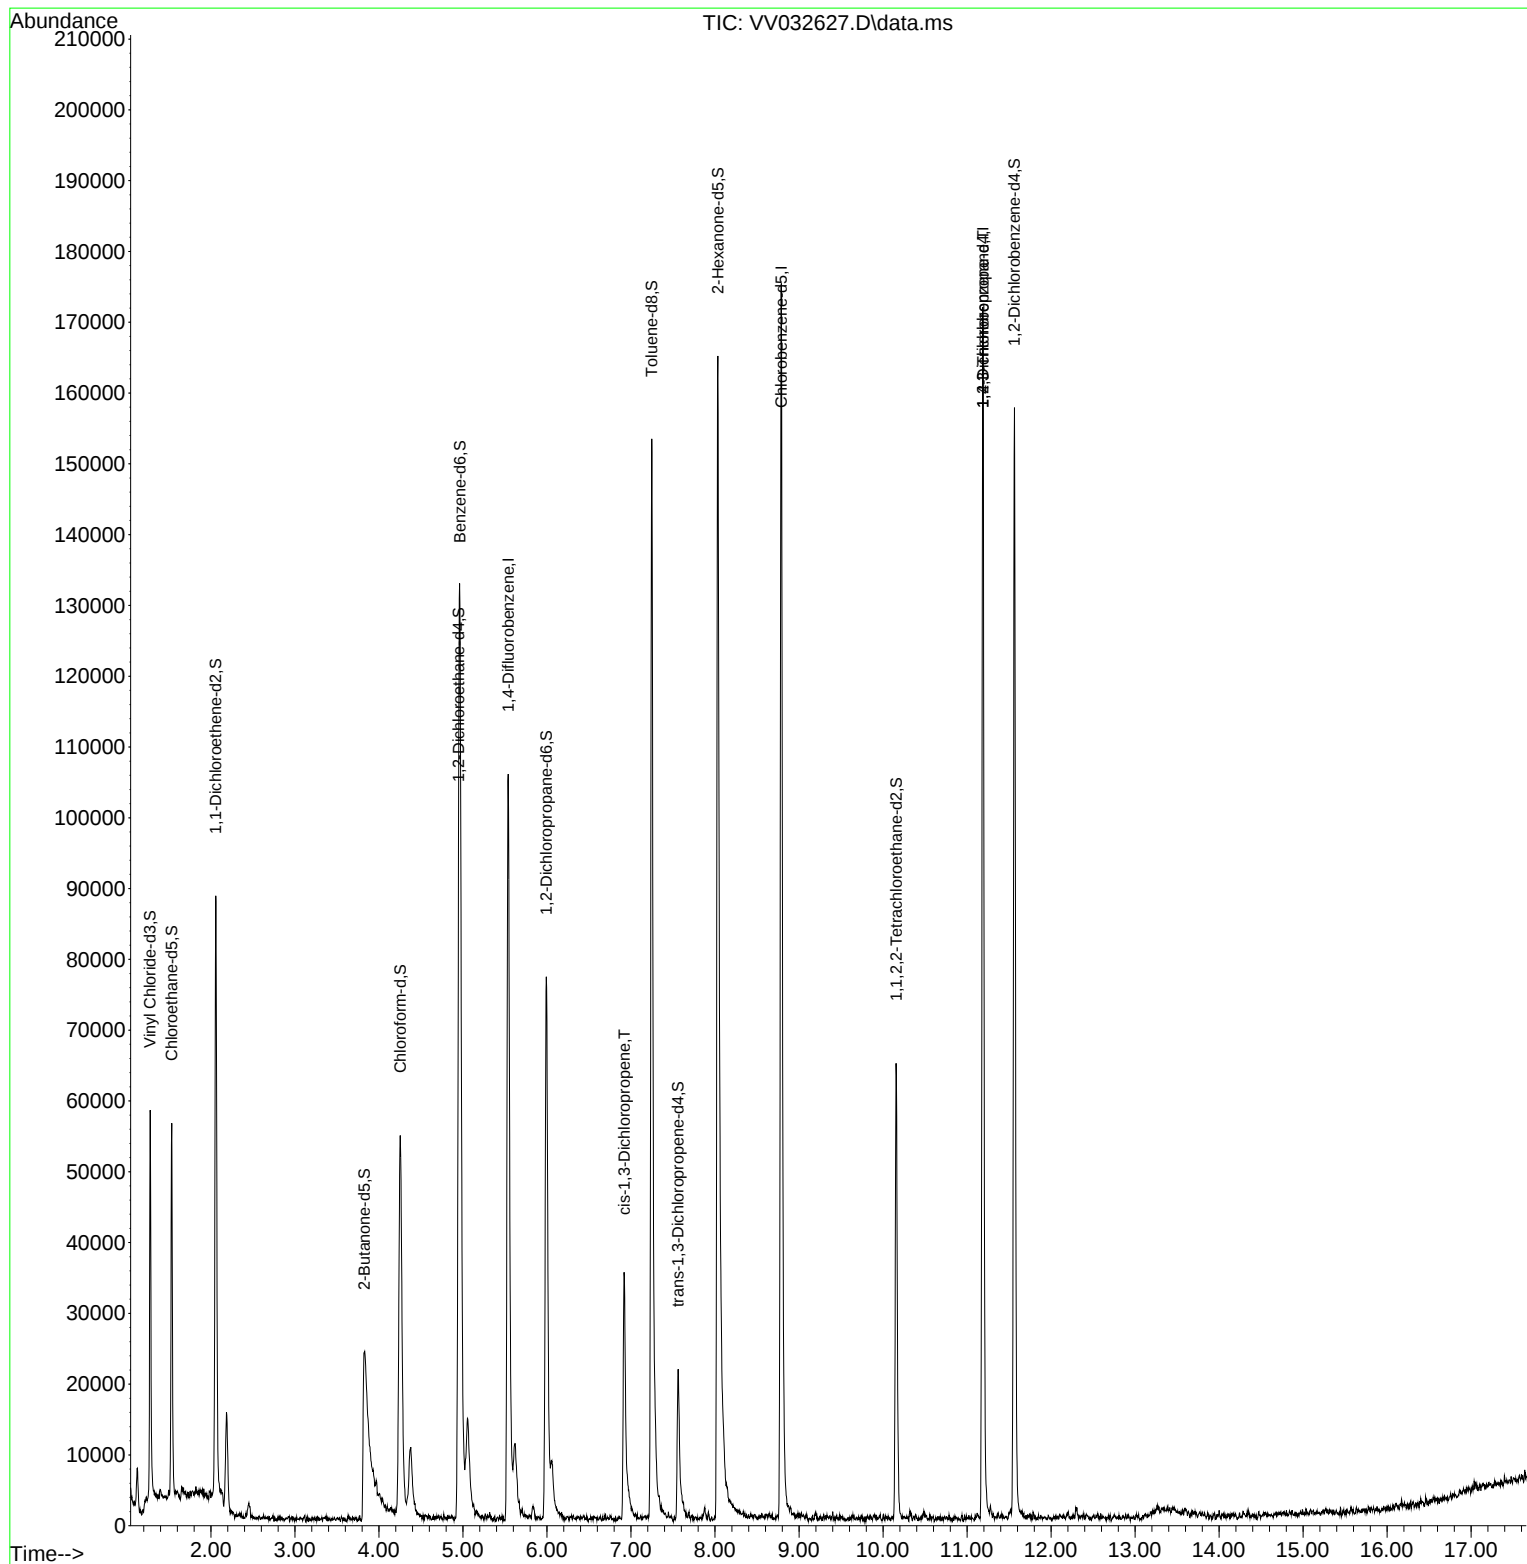

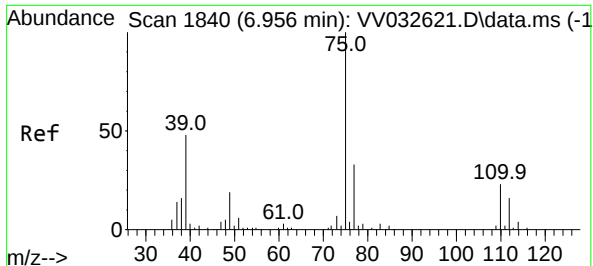

#39

cis-1,3-Dichloropropene

Concen: 0.098 ug/L

RT: 6.921 min Scan# 11

Delta R.T. -0.035 min

Lab File: VV032627.D

Acq: 25 Oct 2023 12:50

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 75 Resp: 1330

Ion Ratio Lower Upper

75 100

77 47.1 22.2 41.2#

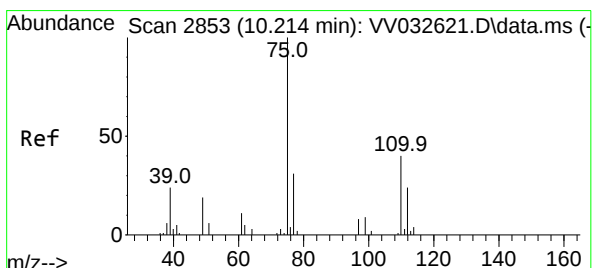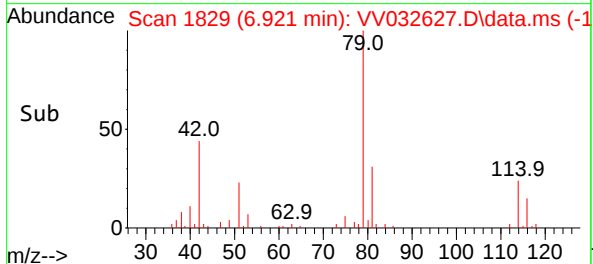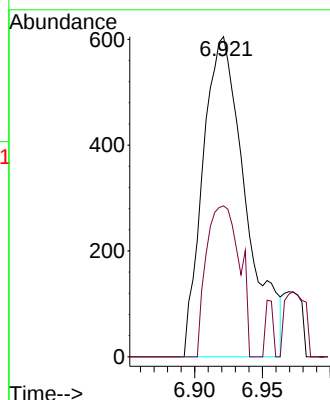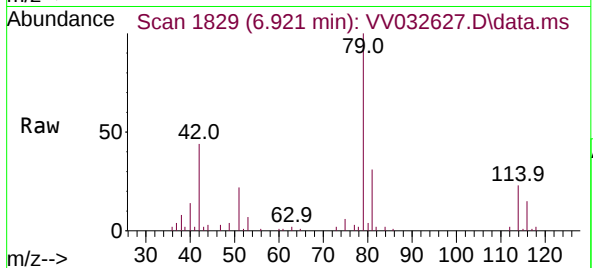

#61

1,2,3-Trichloropropane

Concen: 1.236 ug/L

RT: 11.188 min Scan# 3156

Delta R.T. 0.974 min

Lab File: VV032627.D

Acq: 25 Oct 2023 12:50

Tgt Ion: 75 Resp: 5893

Ion Ratio Lower Upper

75 100

77 33.1 26.2 39.2

110 2.5 30.6 46.0#

