

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102523\
 Data File : VW032644.D
 Acq On : 25 Oct 2023 19:38
 Operator : SY/MD
 Sample : 04961-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 26 05:05:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 26 04:59:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	88267	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	101182	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	43398	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	33511	4.668	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.400%
7) Chloroethane-d5	1.532	69	30794	5.285	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.600%
11) 1,1-Dichloroethene-d2	2.059	65	12937	4.273	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.400%
20) 2-Butanone-d5	3.818	46	51012	28.091	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	56.180%
24) Chloroform-d	4.252	84	58425	4.614	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.200%
26) 1,2-Dichloroethane-d4	4.947	65	30122	5.022	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	4.963	84	114697	3.852	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.000%
36) 1,2-Dichloropropane-d6	5.992	67	36591	3.709	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	74.200%
41) Toluene-d8	7.246	98	103768	3.812	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.200%
43) trans-1,3-Dichloroprop...	7.558	79	13900	3.977	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.600%
46) 2-Hexanone-d5	8.030	63	60088	36.536	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.080%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	31213	4.524	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.400%
66) 1,2-Dichlorobenzene-d4	11.564	152	39313	4.882	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.600%
Target Compounds						
61) 1,2,3-Trichloropropane	11.188	75	5688	1.231	ug/L	Qvalue # 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032644.D
Acq On : 25 Oct 2023 19:38
Operator : SY/MD
Sample : 04961-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 26 05:05:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 26 04:59:52 2023
Response via : Initial Calibration

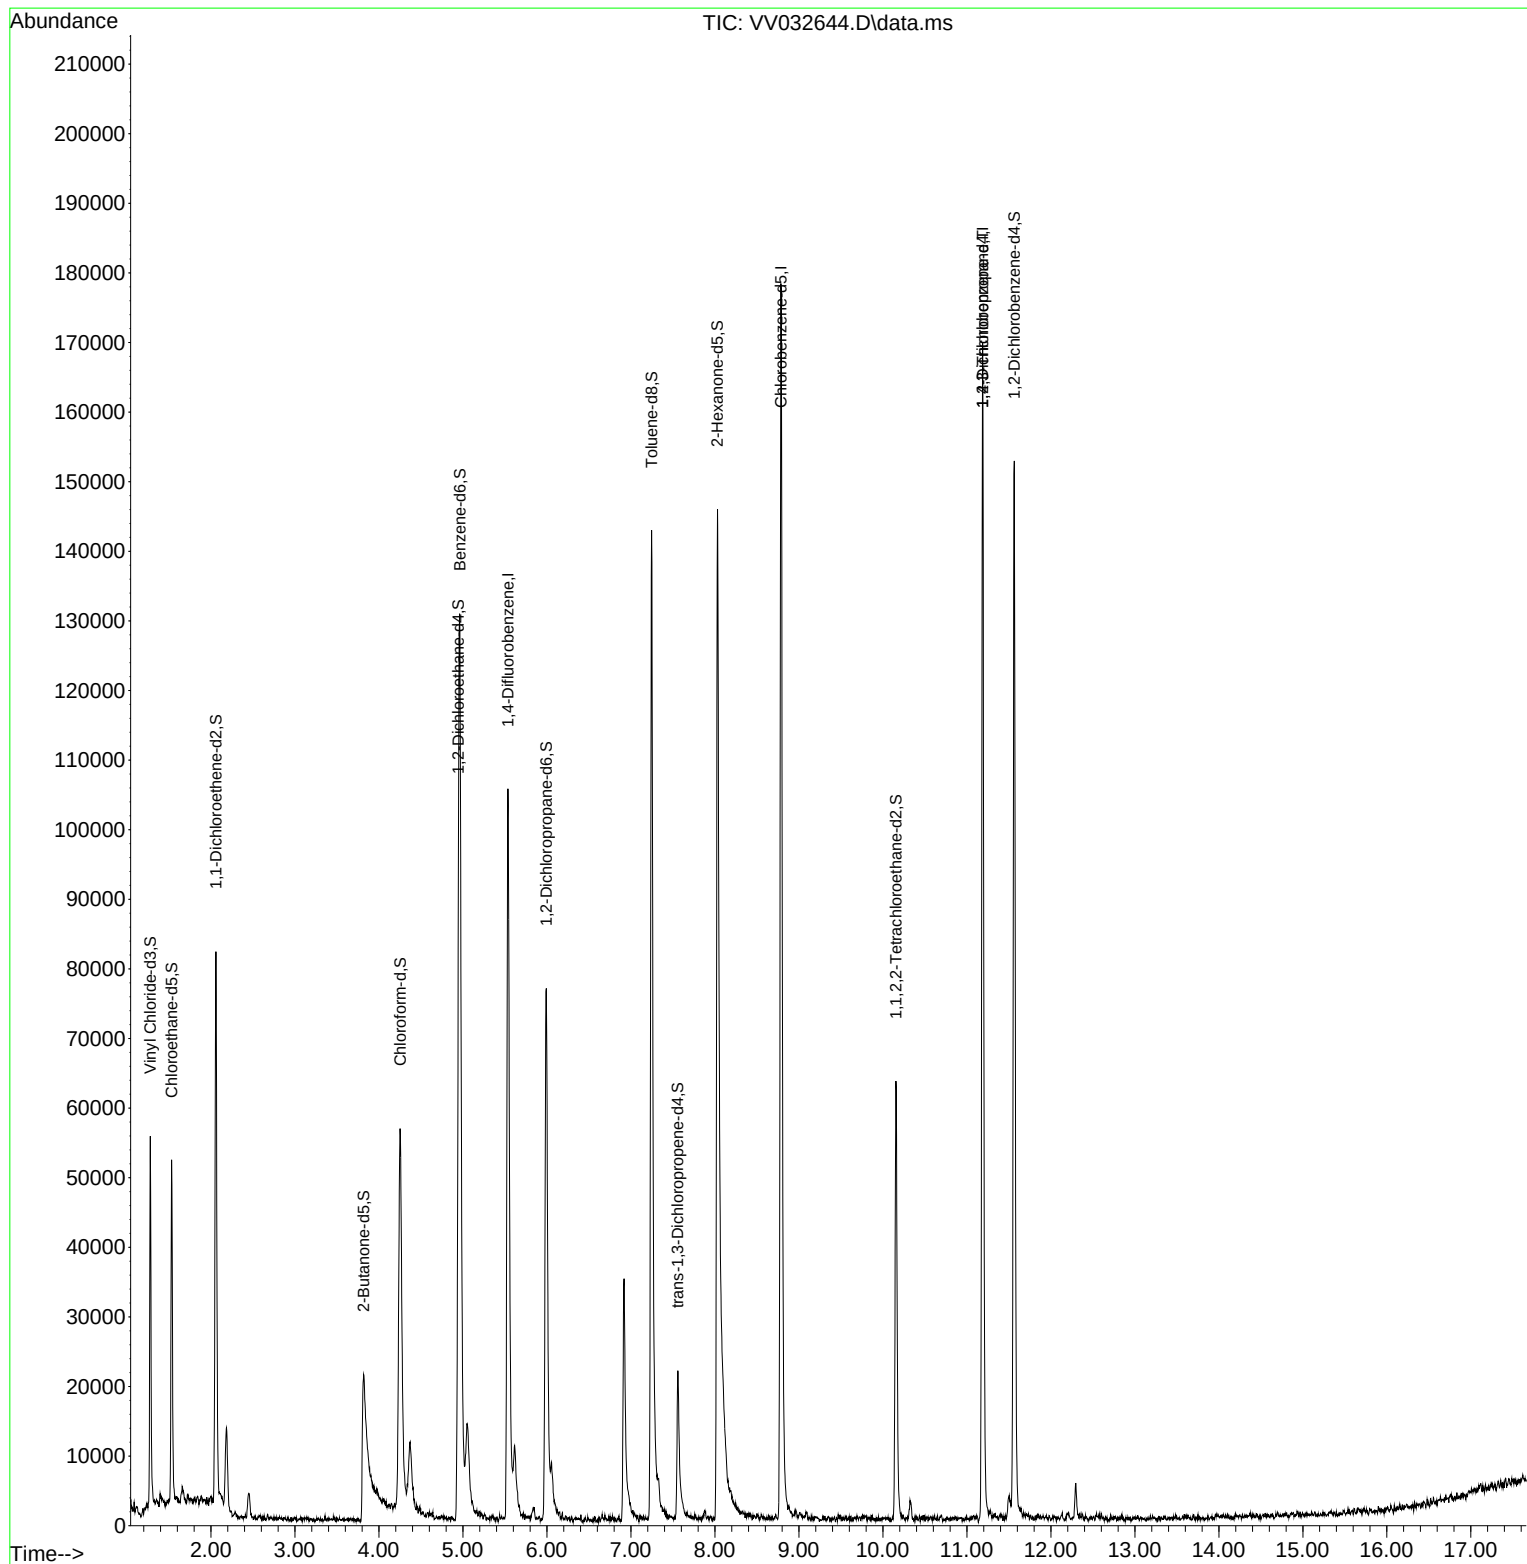

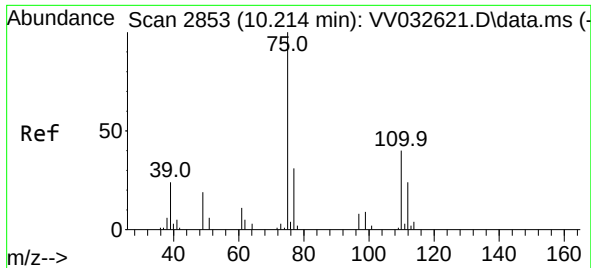

#61
 1,2,3-Trichloropropane
 Concen: 1.231 ug/L
 RT: 11.188 min Scan# 31
 Delta R.T. 0.974 min
 Lab File: VV032644.D
 Acq: 25 Oct 2023 19:38

Instrument :
 MSVOA_V
 ClientSampleId :

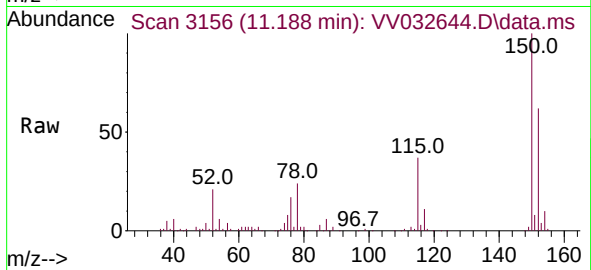

Tgt Ion: 75 Resp: 5688
 Ion Ratio Lower Upper
 75 100
 77 31.6 26.2 39.2
 110 1.1 30.6 46.0#

