




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
 Data File : VV032623.D
 Acq On : 25 Oct 2023 11:15
 Operator : SY/MD
 Sample : 04992-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK7

Manual IntegrationsAPPROVED

Quant Time: Oct 26 05:01:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 26 04:59:52 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/26/2023
 Supervised By :Mahesh Dadoda 10/27/2023

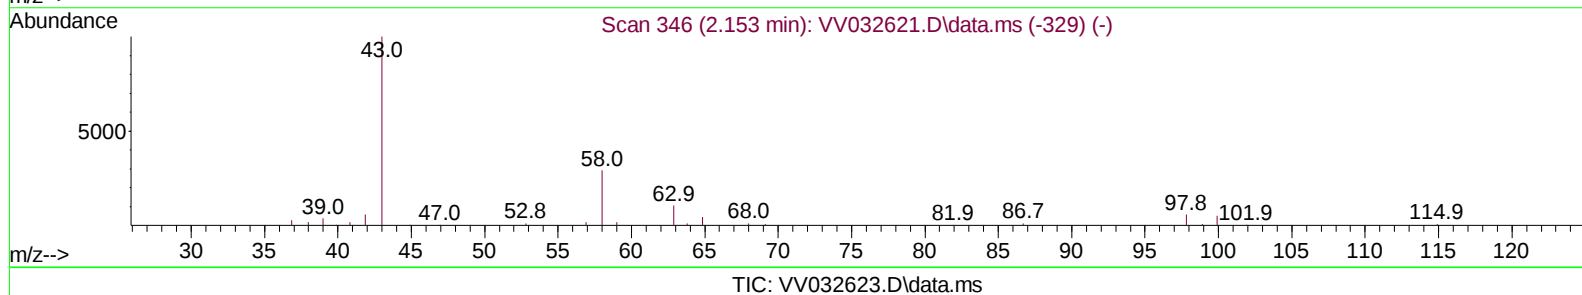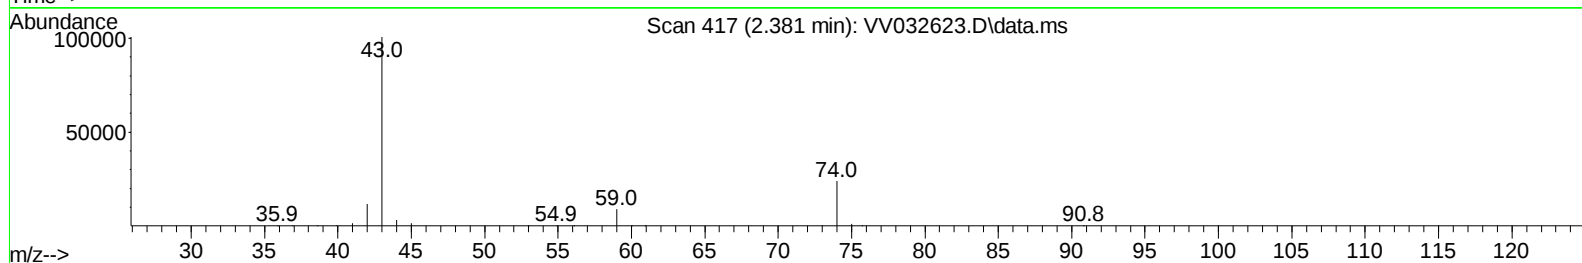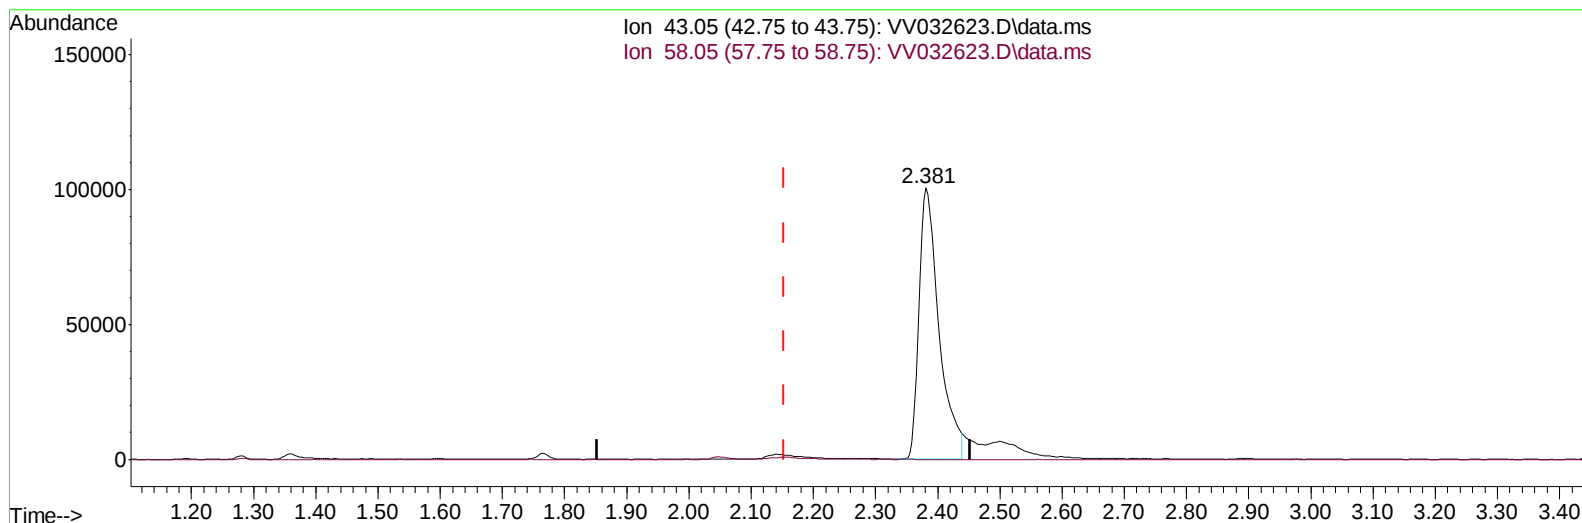

(13) Acetone (T)

2.381min (+ 0.228) 148.83 ug/L

response 224683

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.00	0.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
 Data File : VV032623.D
 Acq On : 25 Oct 2023 11:15
 Operator : SY/MD
 Sample : 04992-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK7

Manual IntegrationsAPPROVED

Quant Time: Oct 26 05:01:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 26 04:59:52 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/26/2023
 Supervised By :Mahesh Dadoda 10/27/2023

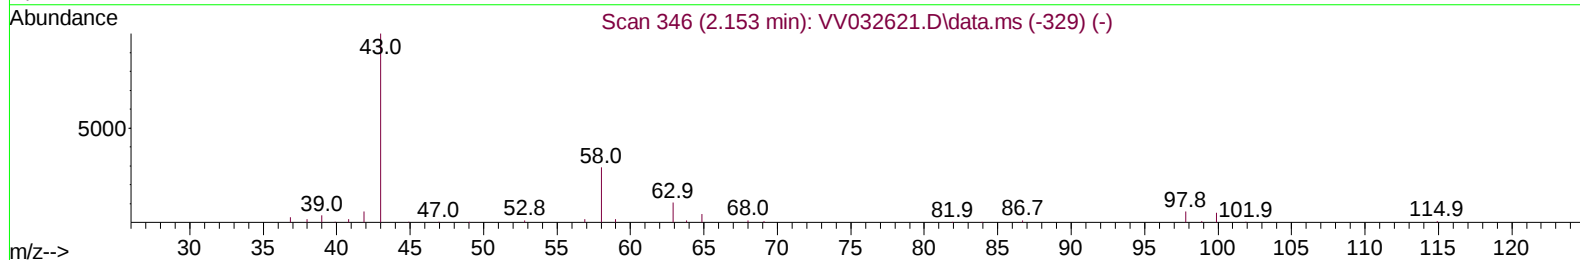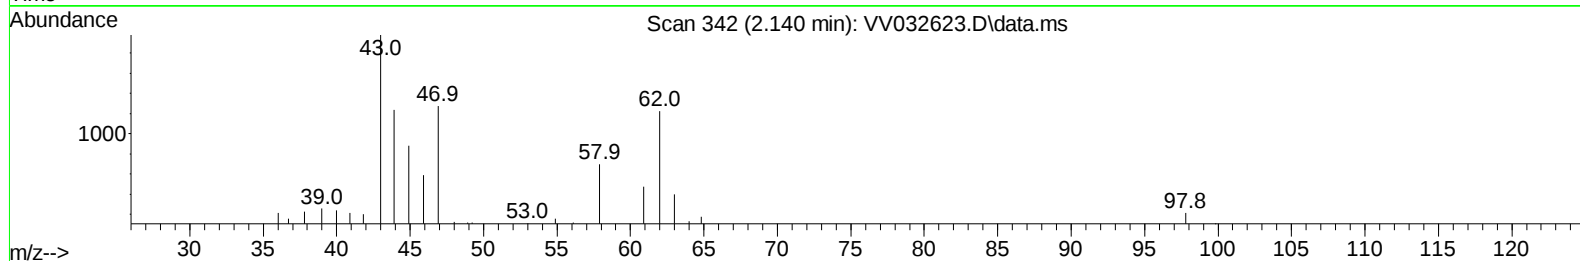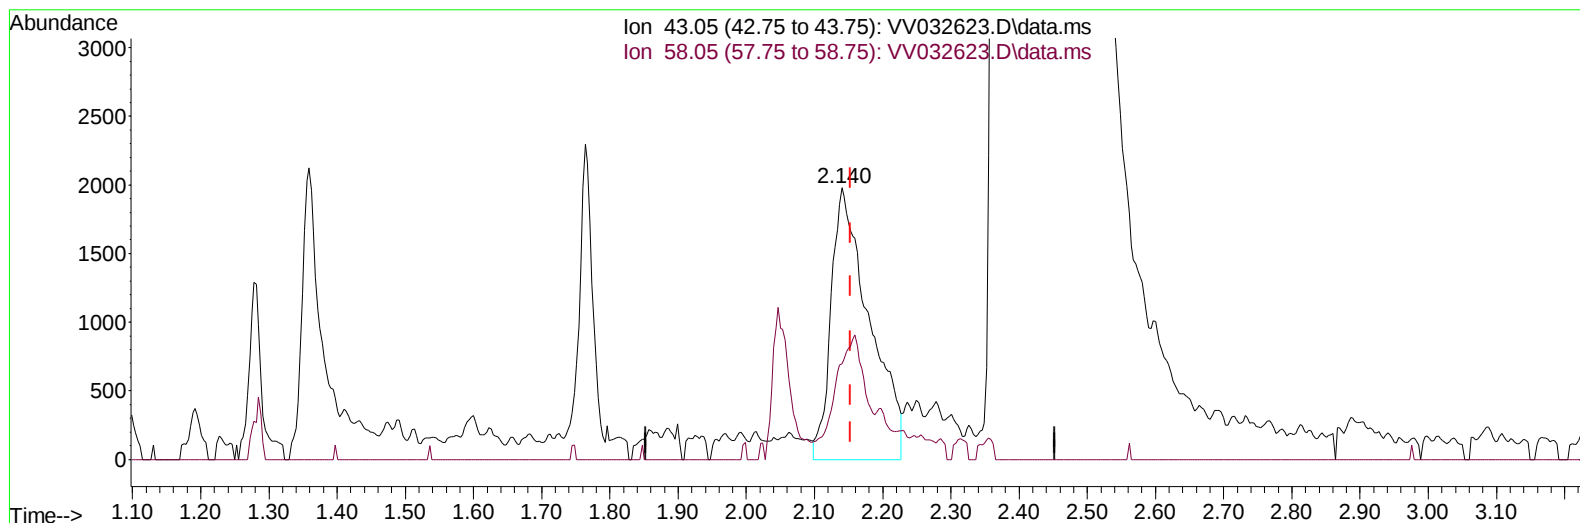

TIC: VV032623.D\data.ms

(13) Acetone (T)

2.140min (-0.013) 5.10 ug/L m

response 7696

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.00	2.47
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
 Data File : VV032623.D
 Acq On : 25 Oct 2023 11:15
 Operator : SY/MD
 Sample : 04992-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK7

Manual IntegrationsAPPROVED

Quant Time: Oct 26 05:01:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 26 04:59:52 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/26/2023
 Supervised By :Mahesh Dadoda 10/27/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	95205	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	95107	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	43629	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	21292	2.750	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	55.000%	
7) Chloroethane-d5	1.532	69	22899	3.643	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	72.800%	
11) 1,1-Dichloroethene-d2	2.060	65	9036	2.767	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	55.400%#	
20) 2-Butanone-d5	3.809	46	83949	42.860	ug/L	-0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	85.720%	
24) Chloroform-d	4.249	84	51779	3.791	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	75.800%	
26) 1,2-Dichloroethane-d4	4.947	65	27386	4.233	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	84.600%	
32) Benzene-d6	4.963	84	90088	3.219	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	64.400%#	
36) 1,2-Dichloropropane-d6	5.992	67	35036	3.779	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	75.600%	
41) Toluene-d8	7.246	98	74682	2.918	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	58.400%#	
43) trans-1,3-Dichloroprop...	7.558	79	10177	3.097	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	62.000%	
46) 2-Hexanone-d5	8.030	63	68354	44.216	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	88.440%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	29966	4.621	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	92.400%	
66) 1,2-Dichlorobenzene-d4	11.564	152	33648	4.156	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	83.200%	
Target Compounds						
5) Vinyl chloride	1.282	62	2239	0.219	ug/L	90
13) Acetone	2.140	43	7696m	5.098	ug/L	
14) Carbon disulfide	2.243	76	7519	0.308	ug/L	97
15) Methyl Acetate	2.381	43	239418	70.446	ug/L	98
21) 2-Butanone	3.915	43	15445	6.542	ug/L	87
22) cis-1,2-Dichloroethene	3.815	96	155456	18.052	ug/L	97
47) Tetrachloroethene	7.911	164	6713	0.968	ug/L	89
63) 1,2,4-Trimethylbenzene	10.857	105	2263	0.082	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032623.D
Acq On : 25 Oct 2023 11:15
Operator : SY/MD
Sample : 04992-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK7

Manual IntegrationsAPPROVED

Quant Time: Oct 26 05:01:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 26 04:59:52 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/26/2023
Supervised By :Mahesh Dadoda 10/27/2023

