

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102523\
 Data File : VW032643.D
 Acq On : 25 Oct 2023 19:14
 Operator : SY/MD
 Sample : 04948-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Quant Time: Oct 26 05:05:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 26 04:59:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	86361	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	98355	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	42589	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	33222	4.730	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	94.600%	
7) Chloroethane-d5	1.532	69	30845	5.410	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	108.200%	
11) 1,1-Dichloroethene-d2	2.060	65	13327	4.499	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	90.000%	
20) 2-Butanone-d5	3.809	46	53692	30.219	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	60.440%	
24) Chloroform-d	4.253	84	57976	4.679	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.600%	
26) 1,2-Dichloroethane-d4	4.947	65	30728	5.236	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.800%	
32) Benzene-d6	4.963	84	115432	3.989	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	79.800%	
36) 1,2-Dichloropropane-d6	5.992	67	36932	3.852	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	77.000%	
41) Toluene-d8	7.246	98	105976	4.005	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	80.000%	
43) trans-1,3-Dichloroprop...	7.561	79	13422	3.950	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	79.000%	
46) 2-Hexanone-d5	8.030	63	62749	39.250	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	78.500%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	31431	4.686	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.800%	
66) 1,2-Dichlorobenzene-d4	11.564	152	39461	4.993	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	8986	1.088	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032643.D
Acq On : 25 Oct 2023 19:14
Operator : SY/MD
Sample : 04948-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Time: Oct 26 05:05:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 26 04:59:52 2023
Response via : Initial Calibration

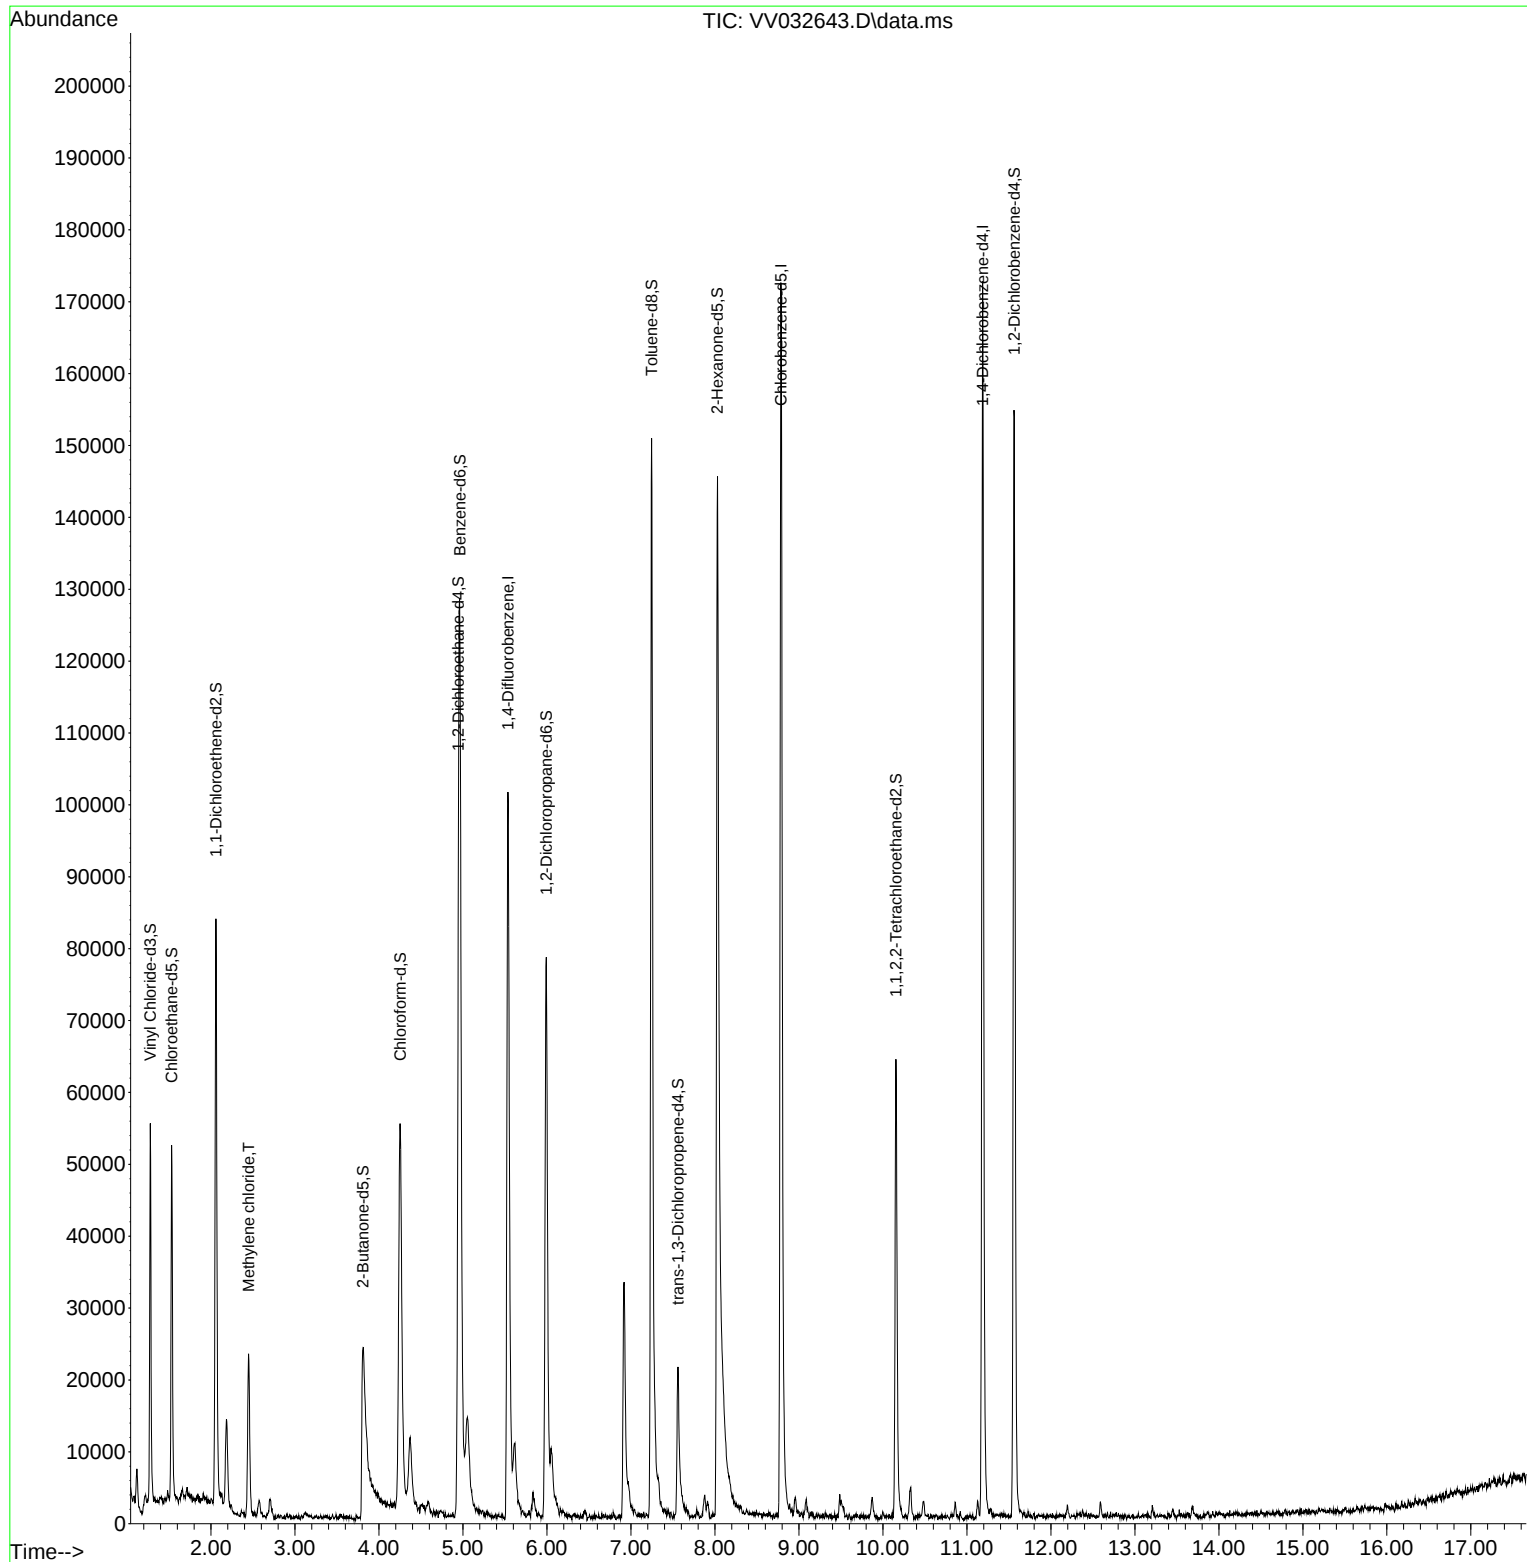

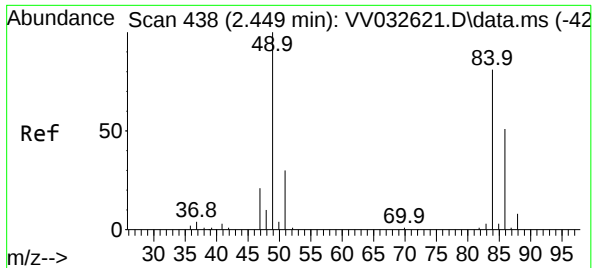

#16
Methylene chloride
Concen: 1.088 ug/L
RT: 2.449 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV032643.D
Acq: 25 Oct 2023 19:14

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Tgt Ion:	84	Resp:	8986
Ion	Ratio	Lower	Upper
84	100		
86	68.1	43.2	80.2
49	129.5	86.3	160.3

