

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
 Data File : VV032622.D
 Acq On : 25 Oct 2023 10:47
 Operator : SY/MD
 Sample : VV1025WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK380

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	17	23	32	rVB	5372	7588	2.30%	0.269%
2	1.278	67	74	85	rVB	54271	56859	17.23%	2.012%
3	1.532	146	153	163	rBV	50792	59580	18.06%	2.108%
4	2.060	307	317	331	rBV	84353	121383	36.79%	4.295%
5	2.179	342	354	365	rVB2	11332	23609	7.16%	0.835%
6	3.818	854	864	883	rBV	19885	67115	20.34%	2.375%
7	4.253	983	999	1020	rBV2	53266	140337	42.53%	4.966%
8	4.365	1022	1034	1045	rVB4	6882	17546	5.32%	0.621%
9	4.960	1204	1219	1237	rBV3	127946	329939	100.00%	11.675%
10	5.539	1387	1399	1414	rBV	100418	209363	63.46%	7.408%
11	5.992	1526	1540	1553	rBV	75807	161491	48.95%	5.714%
12	6.918	1818	1828	1856	rBV	34861	75863	22.99%	2.684%
13	7.246	1919	1930	1956	rBV	148227	289653	87.79%	10.250%
14	7.558	2018	2027	2046	rBV2	20046	40166	12.17%	1.421%
15	8.031	2165	2174	2210	rBV	128572	316458	95.91%	11.198%
16	8.786	2398	2409	2429	rBV	167904	301169	91.28%	10.657%
17	10.156	2818	2835	2854	rBV	57688	98367	29.81%	3.481%
18	11.188	3145	3156	3177	rBV	160073	260900	79.08%	9.232%
19	11.564	3260	3273	3290	rBV	151723	245141	74.30%	8.674%
20	13.452	3856	3860	3871	rVB6	2487	3471	1.05%	0.123%




Sum of corrected areas: 2825998

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032622.D
Acq On : 25 Oct 2023 10:47
Operator : SY/MD
Sample : VV1025WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

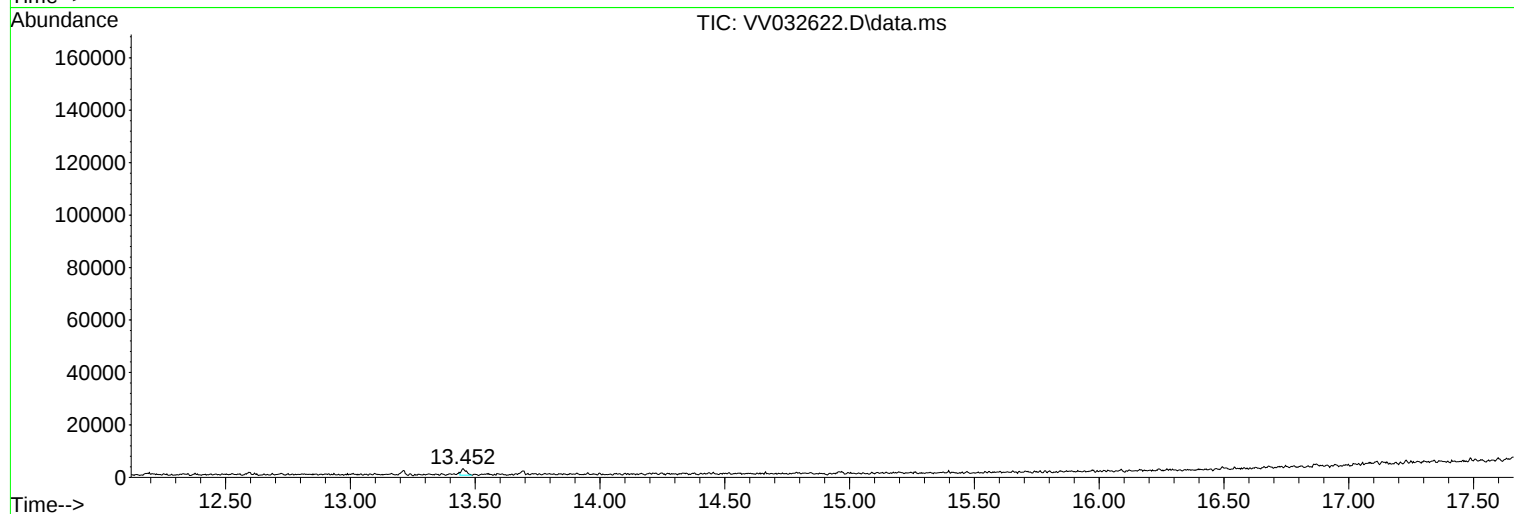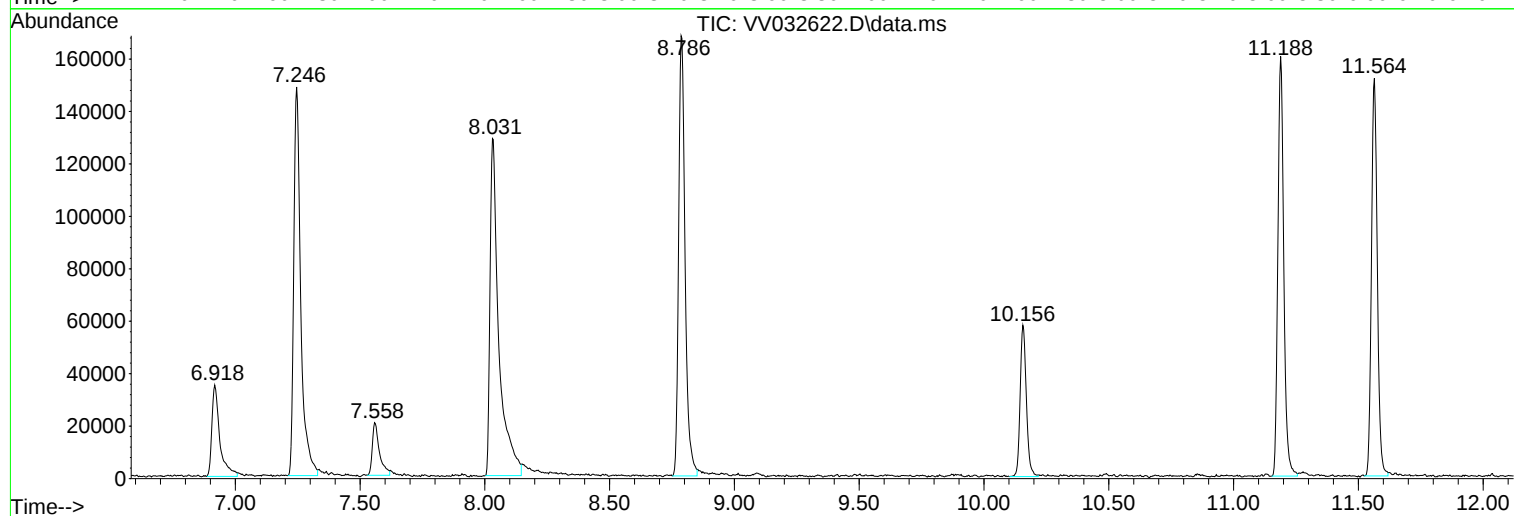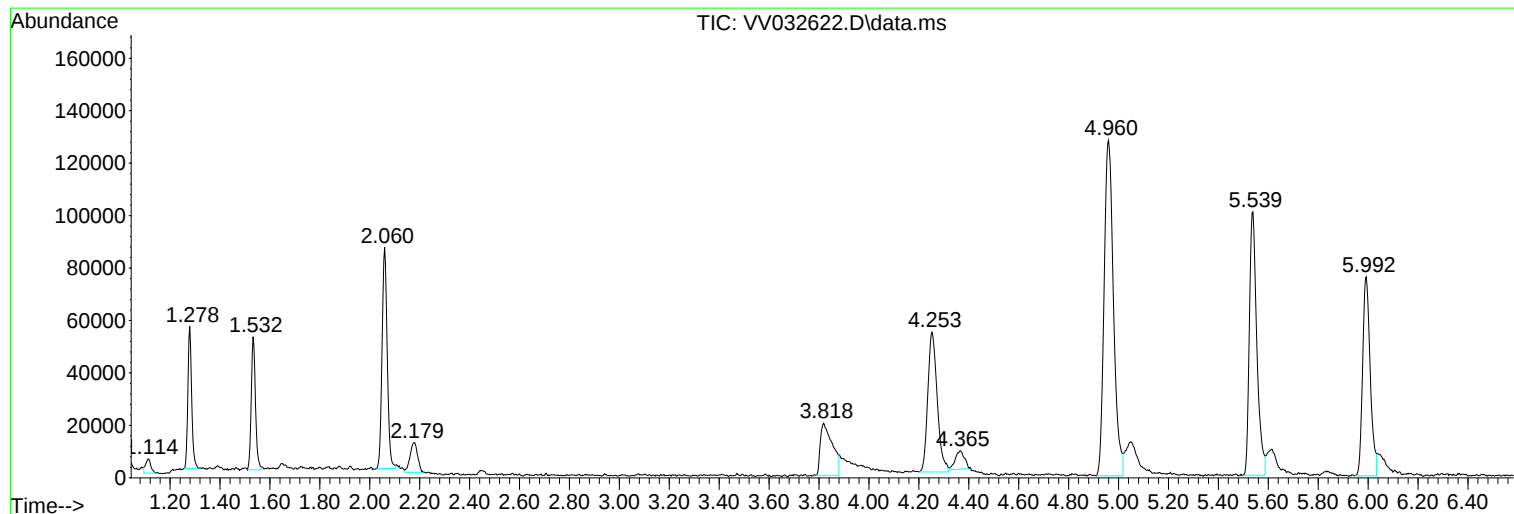

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032622.D
Acq On : 25 Oct 2023 10:47
Operator : SY/MD
Sample : VV1025WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032622.D
Acq On : 25 Oct 2023 10:47
Operator : SY/MD
Sample : VV1025WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
