

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
 Data File : VV032623.D
 Acq On : 25 Oct 2023 11:15
 Operator : SY/MD
 Sample : 04992-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	17	rBV	16156	15317	1.95%	0.374%
2	1.278	65	74	83	rBV2	43514	53947	6.88%	1.317%
3	1.362	93	100	103	rBV	6284	8246	1.05%	0.201%
4	1.536	146	154	165	rVB	37371	43764	5.58%	1.068%
5	2.060	307	317	332	rBV	55761	84824	10.81%	2.071%
6	2.159	336	348	364	rVV5	25642	55197	7.04%	1.347%
7	2.243	367	374	395	rVB	6960	15923	2.03%	0.389%
8	2.381	403	417	447	rBV	152360	367889	46.89%	8.980%
9	3.815	848	863	884	rBV2	305661	784528	100.00%	19.150%
10	3.928	891	898	928	rVB3	38312	111896	14.26%	2.731%
11	4.249	982	998	1019	rBV2	46882	125092	15.94%	3.053%
12	4.359	1022	1032	1046	rVB3	6069	15241	1.94%	0.372%
13	4.960	1203	1219	1236	rBV3	104300	270300	34.45%	6.598%
14	5.535	1386	1398	1415	rBV	98251	209772	26.74%	5.120%
15	5.992	1523	1540	1555	rBV	67876	146493	18.67%	3.576%
16	6.918	1815	1828	1848	rBV2	26779	55185	7.03%	1.347%
17	7.246	1918	1930	1950	rBV	103021	200896	25.61%	4.904%
18	7.458	1986	1996	2006	rBV	8681	16840	2.15%	0.411%
19	7.561	2020	2028	2044	rBV3	15475	31392	4.00%	0.766%
20	7.908	2126	2136	2148	rBV2	28427	50185	6.40%	1.225%
21	8.030	2164	2174	2207	rBV	186407	404703	51.59%	9.879%
22	8.786	2399	2409	2433	rBV	165074	293764	37.44%	7.171%
23	9.066	2489	2496	2513	rVB7	8260	16179	2.06%	0.395%
24	9.657	2669	2680	2691	rBV5	6006	10768	1.37%	0.263%
25	10.156	2820	2835	2852	rBV	64773	109644	13.98%	2.676%
26	10.390	2901	2908	2922	rBV9	5301	10586	1.35%	0.258%
27	10.985	3086	3093	3103	rBV	13310	23229	2.96%	0.567%
28	11.188	3146	3156	3174	rVV	174319	273446	34.85%	6.675%
29	11.278	3174	3184	3193	rVB4	7435	12426	1.58%	0.303%
30	11.497	3239	3252	3262	rBV8	10145	27320	3.48%	0.667%
31	11.564	3262	3273	3289	rVB	134164	225684	28.77%	5.509%
32	12.181	3456	3465	3477	rBV3	14355	26070	3.32%	0.636%




Sum of corrected areas: 4096746

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032623.D
Acq On : 25 Oct 2023 11:15
Operator : SY/MD
Sample : 04992-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

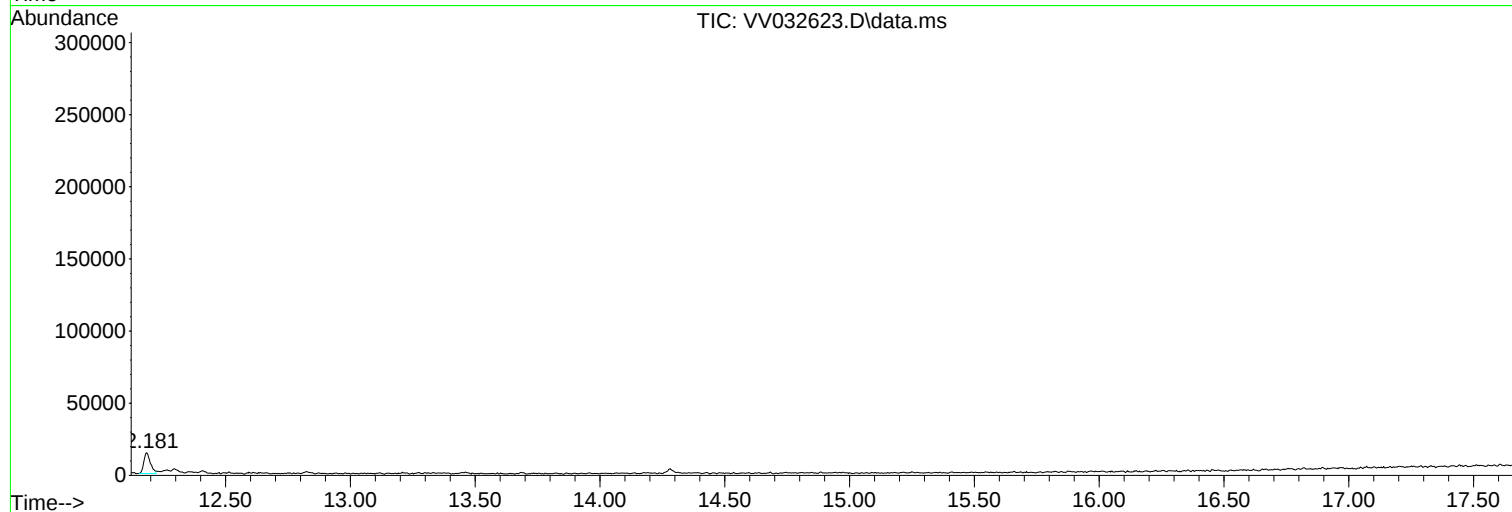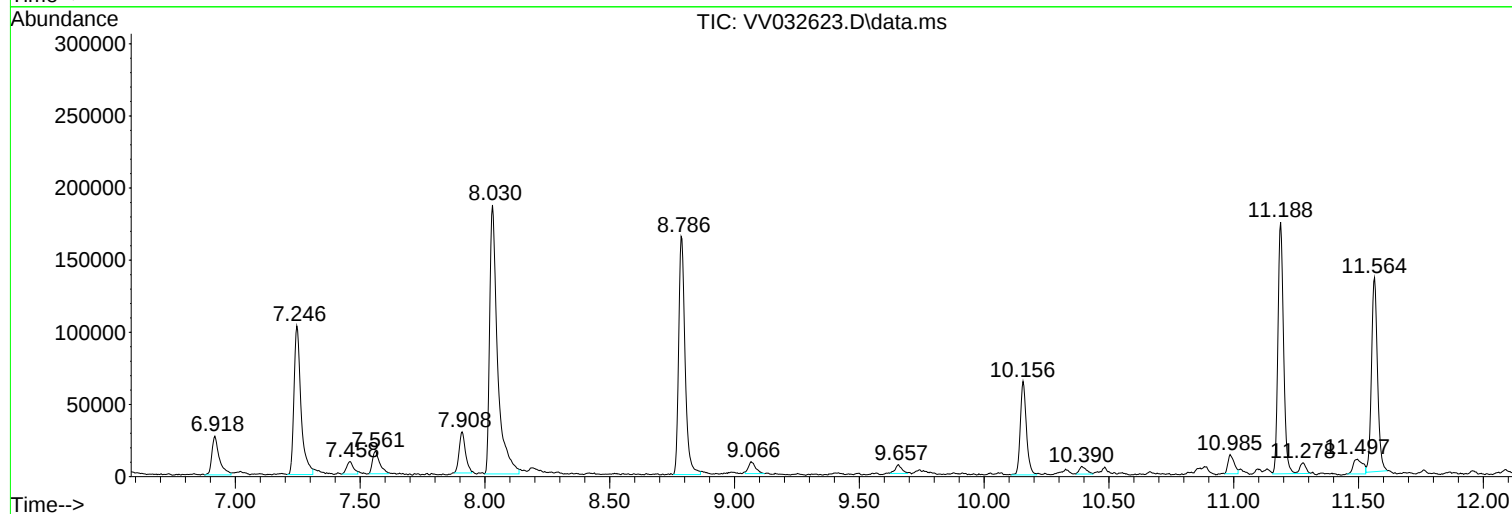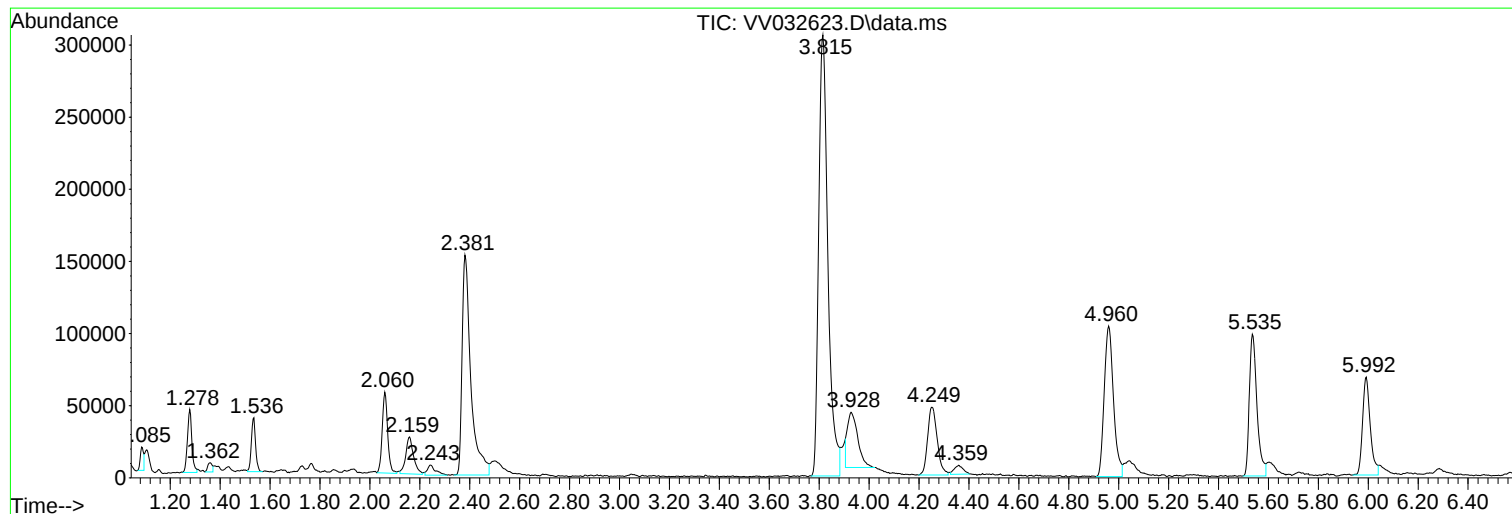

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032623.D
Acq On : 25 Oct 2023 11:15
Operator : SY/MD
Sample : 04992-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032623.D
Acq On : 25 Oct 2023 11:15
Operator : SY/MD
Sample : 04992-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc