

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
 Data File : VV032626.D
 Acq On : 25 Oct 2023 12:26
 Operator : SY/MD
 Sample : 04950-25
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4A16

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	65	74	87	rBV	52918	58265	15.51%	1.882%
2	1.535	147	154	165	rVB	46903	57249	15.24%	1.849%
3	2.059	307	317	330	rBV	79914	117434	31.27%	3.793%
4	2.185	345	356	368	rVB	12286	24755	6.59%	0.800%
5	3.812	852	862	889	rBV2	32640	119527	31.82%	3.861%
6	4.256	984	1000	1024	rBV2	52915	146455	38.99%	4.731%
7	4.374	1025	1037	1053	rVB2	8379	24628	6.56%	0.796%
8	4.960	1203	1219	1239	rBV3	127960	331251	88.20%	10.700%
9	5.056	1243	1249	1267	rVB4	12050	27462	7.31%	0.887%
10	5.538	1388	1399	1416	rBV	110204	229733	61.17%	7.421%
11	5.612	1418	1422	1439	rVB2	9376	20335	5.41%	0.657%
12	5.992	1528	1540	1555	rBV	75769	162202	43.19%	5.239%
13	6.918	1818	1828	1860	rBV	34725	75068	19.99%	2.425%
14	7.246	1919	1930	1964	rBV	146614	290262	77.28%	9.376%
15	7.561	2019	2028	2039	rBV2	19638	37705	10.04%	1.218%
16	8.030	2163	2174	2219	rBV	170767	375589	100.00%	12.132%
17	8.789	2398	2410	2428	rBV	184246	323582	86.15%	10.452%
18	10.156	2824	2835	2853	rBV	63124	103351	27.52%	3.338%
19	11.188	3143	3156	3175	rBV	186019	290569	77.36%	9.386%
20	11.500	3242	3253	3261	rBV6	6740	14097	3.75%	0.455%
21	11.564	3261	3273	3286	rVV	154621	247404	65.87%	7.992%
22	12.291	3491	3499	3513	rBV7	10430	18866	5.02%	0.609%




Sum of corrected areas: 3095789

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032626.D
Acq On : 25 Oct 2023 12:26
Operator : SY/MD
Sample : 04950-25
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

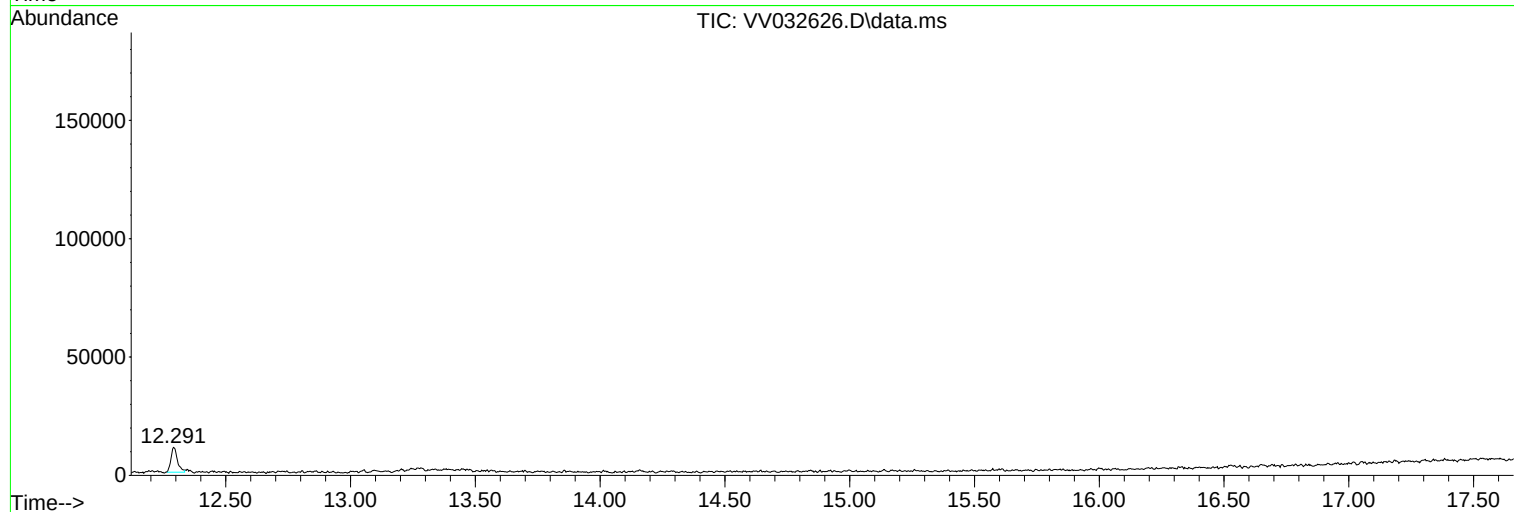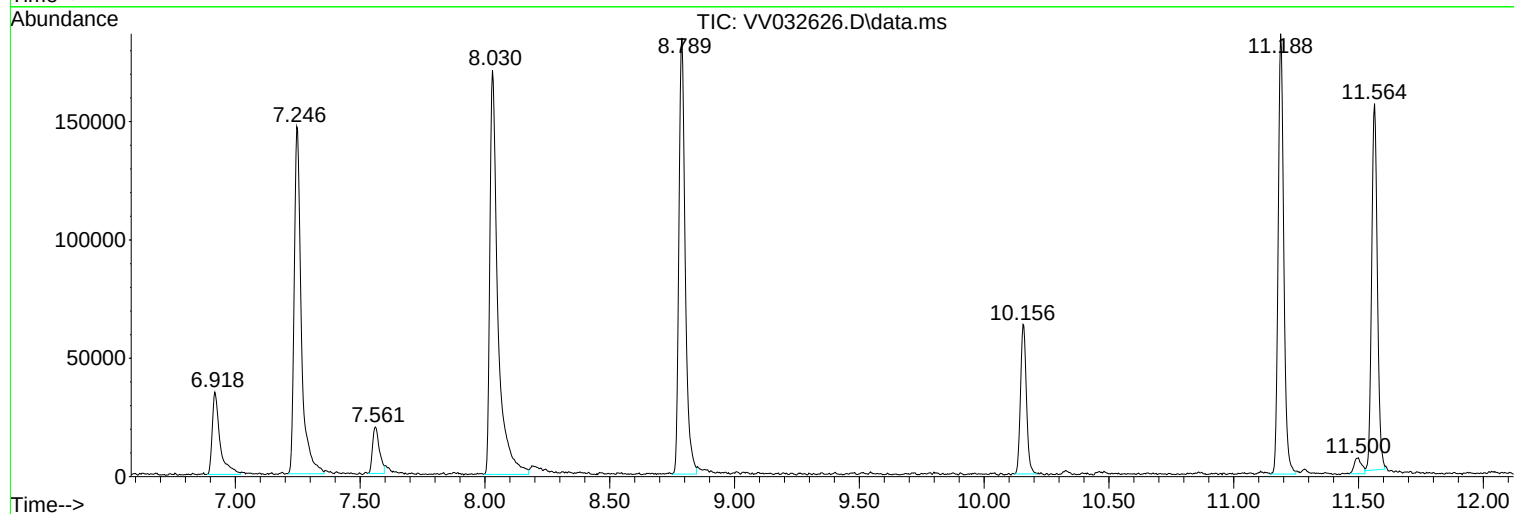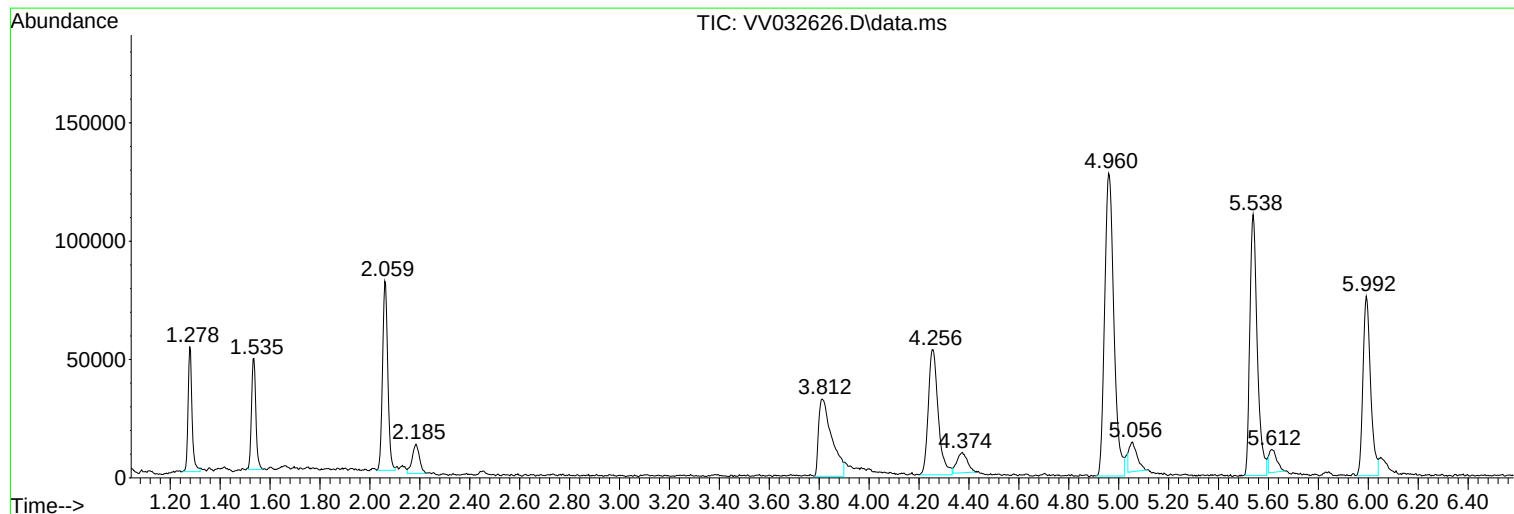

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032626.D
Acq On : 25 Oct 2023 12:26
Operator : SY/MD
Sample : 04950-25
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032626.D
Acq On : 25 Oct 2023 12:26
Operator : SY/MD
Sample : 04950-25
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc