

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
 Data File : VV032627.D
 Acq On : 25 Oct 2023 12:50
 Operator : SY/MD
 Sample : 04950-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	19	26	34	rVB	6239	9101	2.42%	0.307%
2	1.230	49	59	62	rBV8	2188	3817	1.02%	0.129%
3	1.275	65	73	86	rVV	55008	62394	16.59%	2.103%
4	1.532	145	153	165	rBV	52545	61496	16.35%	2.073%
5	2.056	307	316	333	rVB	84299	122524	32.58%	4.130%
6	2.185	346	356	369	rVB2	14163	27521	7.32%	0.928%
7	4.253	984	999	1022	rBV	53236	140106	37.26%	4.722%
8	4.378	1022	1038	1051	rVB2	8196	22025	5.86%	0.742%
9	4.960	1204	1219	1238	rBV2	132066	336327	89.44%	11.336%
10	5.053	1244	1248	1268	rVB3	12464	27924	7.43%	0.941%
11	5.539	1387	1399	1416	rBV	105431	223226	59.37%	7.524%
12	5.619	1419	1424	1437	rVB5	8524	18231	4.85%	0.614%
13	5.992	1527	1540	1555	rBV	76463	165121	43.91%	5.565%
14	6.918	1818	1828	1863	rBV2	34901	78912	20.99%	2.660%
15	7.246	1919	1930	1956	rBV	152366	294117	78.22%	9.913%
16	7.561	2019	2028	2044	rBV2	21035	42968	11.43%	1.448%
17	8.034	2165	2175	2206	rBV	164151	376022	100.00%	12.674%
18	8.789	2399	2410	2431	rBV	174407	313014	83.24%	10.550%
19	10.156	2825	2835	2856	rVB	64373	107391	28.56%	3.620%
20	11.188	3146	3156	3180	rBV	171113	282215	75.05%	9.512%
21	11.564	3262	3273	3293	rBV	156272	252539	67.16%	8.512%




Sum of corrected areas: 2966991

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032627.D
Acq On : 25 Oct 2023 12:50
Operator : SY/MD
Sample : 04950-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

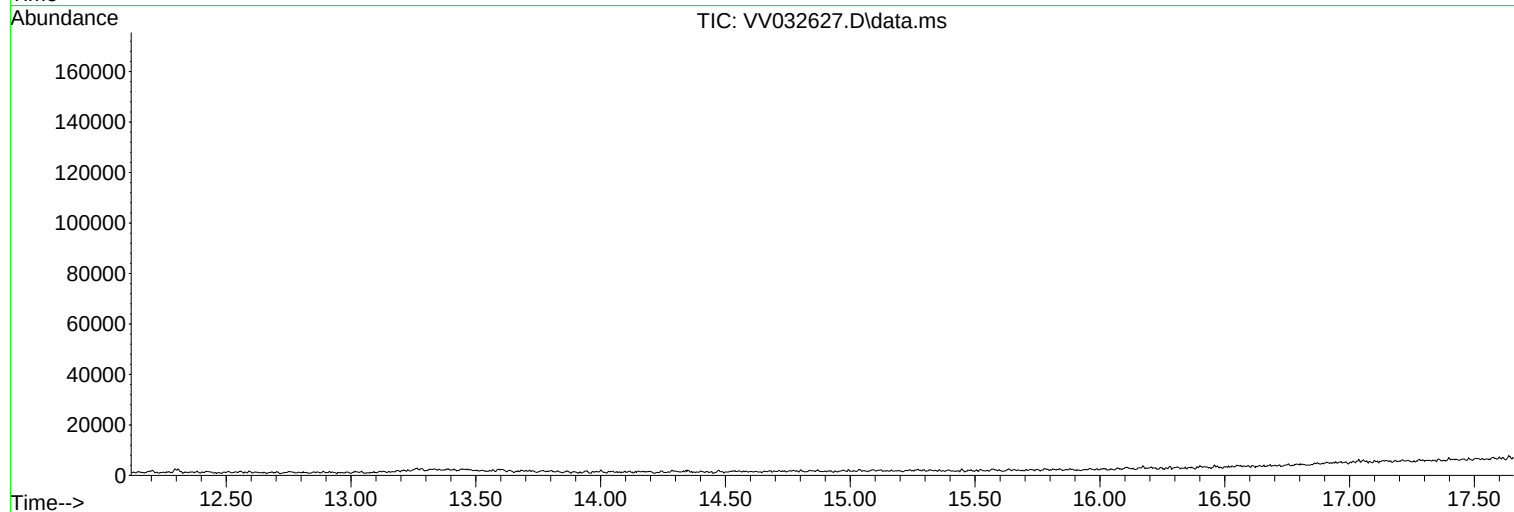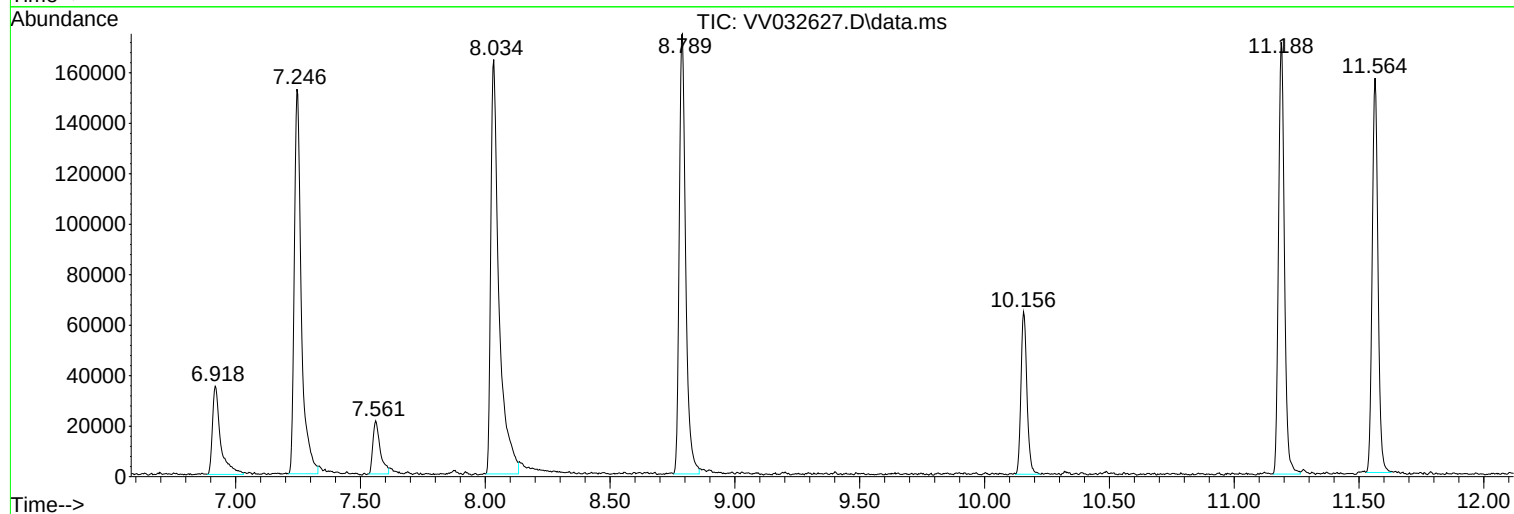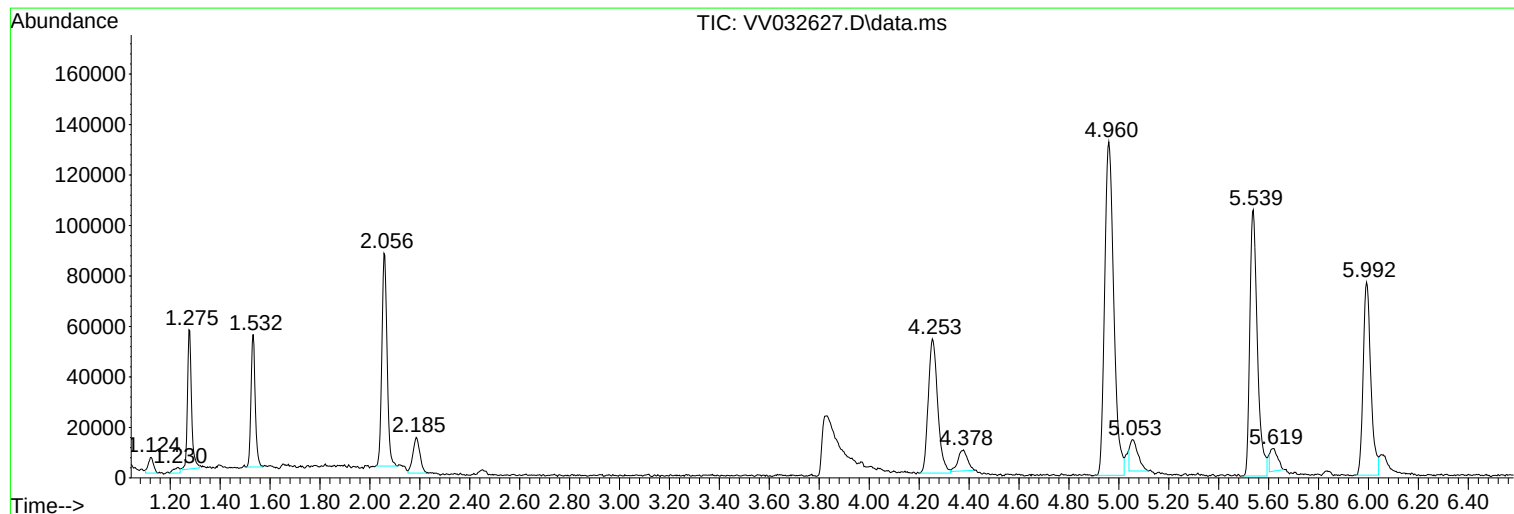

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032627.D
Acq On : 25 Oct 2023 12:50
Operator : SY/MD
Sample : 04950-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032627.D
Acq On : 25 Oct 2023 12:50
Operator : SY/MD
Sample : 04950-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc