

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
 Data File : VV032628.D
 Acq On : 25 Oct 2023 13:14
 Operator : SY/MD
 Sample : 05043-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	20	26	38	rVB	5375	7464	2.01%	0.246%
2	1.278	67	74	87	rBV	56238	59114	15.93%	1.945%
3	1.532	145	153	165	rBV	52413	60604	16.34%	1.994%
4	2.059	307	317	332	rBV	82736	121449	32.74%	3.996%
5	2.188	347	357	369	rVB2	14836	27112	7.31%	0.892%
6	3.818	853	864	897	rBV2	21803	90532	24.40%	2.979%
7	4.252	983	999	1022	rBV2	52925	142285	38.35%	4.681%
8	4.375	1026	1037	1061	rVB4	11693	32987	8.89%	1.085%
9	4.960	1200	1219	1239	rBV4	132286	337899	91.08%	11.117%
10	5.053	1240	1248	1269	rVB5	13450	39874	10.75%	1.312%
11	5.538	1386	1399	1416	rBV	100542	215213	58.01%	7.081%
12	5.619	1416	1424	1437	rVB3	8590	21848	5.89%	0.719%
13	5.992	1520	1540	1554	rBV2	78509	166855	44.98%	5.490%
14	6.918	1817	1828	1842	rBV2	35428	70365	18.97%	2.315%
15	7.246	1919	1930	1958	rBV	148928	293724	79.18%	9.664%
16	7.561	2019	2028	2045	rBV	21212	43339	11.68%	1.426%
17	8.030	2165	2174	2213	rBV	149480	370972	100.00%	12.205%
18	8.789	2400	2410	2438	rBV	170303	304503	82.08%	10.018%
19	10.156	2825	2835	2848	rBV	63656	108162	29.16%	3.559%
20	11.188	3146	3156	3173	rBV	173750	268772	72.45%	8.843%
21	11.564	3261	3273	3288	rBV	157777	256424	69.12%	8.436%




Sum of corrected areas: 3039497

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032628.D
Acq On : 25 Oct 2023 13:14
Operator : SY/MD
Sample : 05043-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

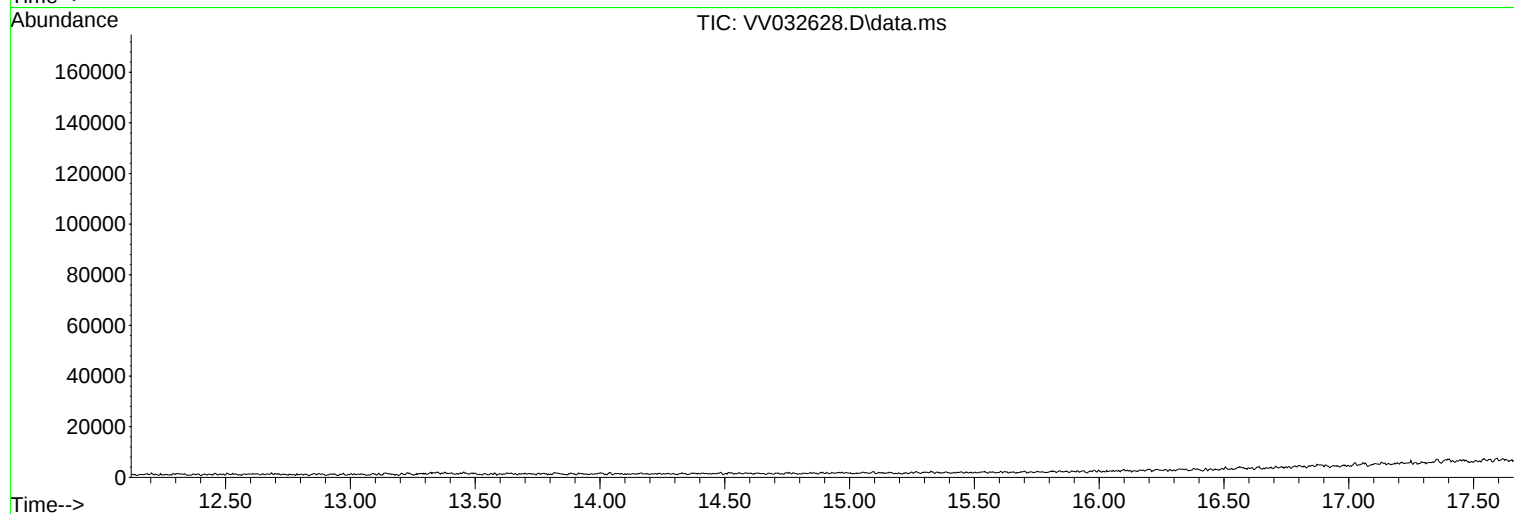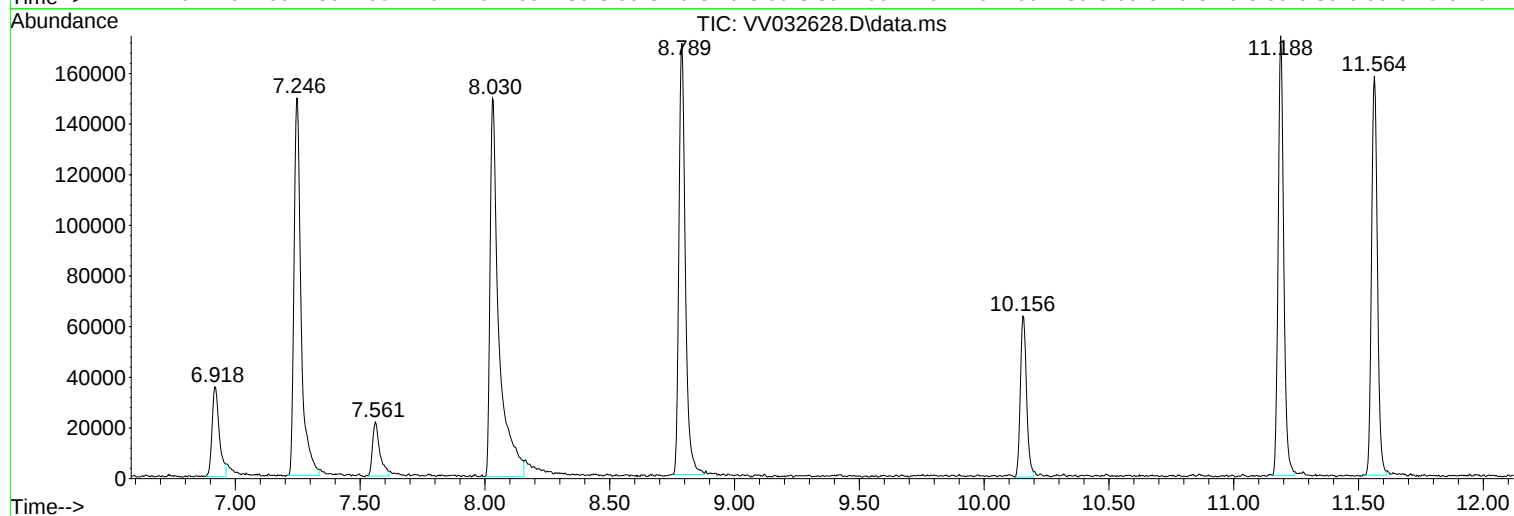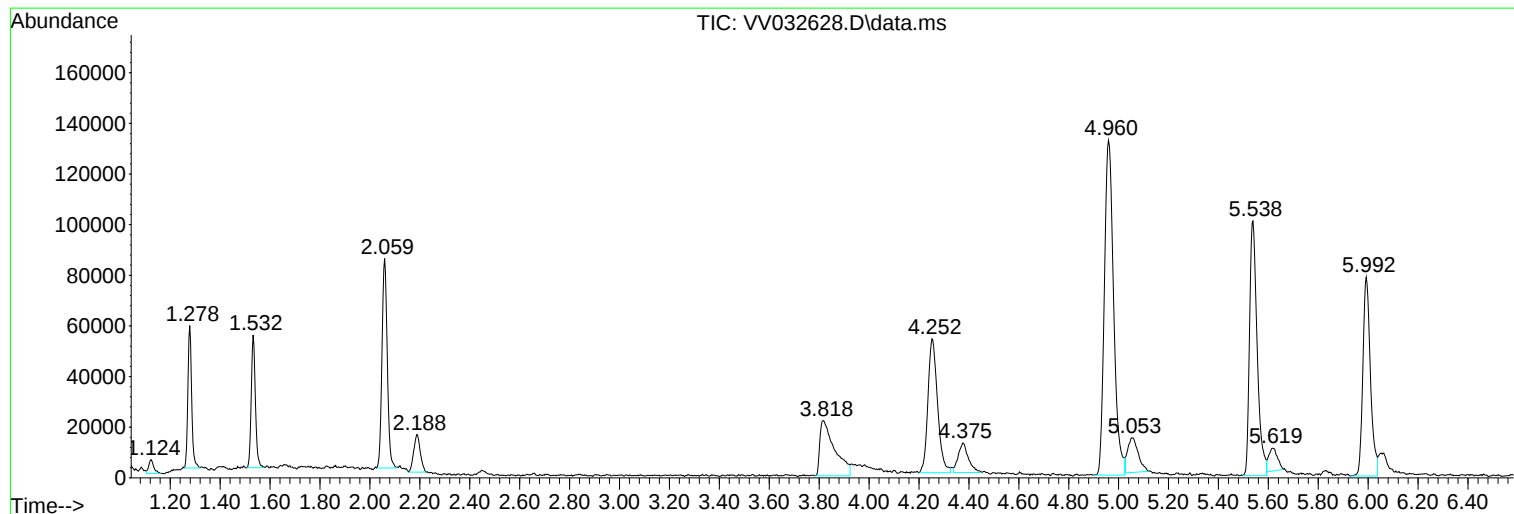

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032628.D
Acq On : 25 Oct 2023 13:14
Operator : SY/MD
Sample : 05043-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032628.D
Acq On : 25 Oct 2023 13:14
Operator : SY/MD
Sample : 05043-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------