

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
 Data File : VV032637.D
 Acq On : 25 Oct 2023 16:48
 Operator : SY/MD
 Sample : 04962-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COALO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	50068	55129	14.20%	1.714%
2	1.532	142	153	166	rBV	49028	60247	15.51%	1.873%
3	2.060	306	317	333	rBV	77169	113833	29.31%	3.539%
4	2.188	347	357	371	rVB2	11924	24531	6.32%	0.763%
5	2.449	430	438	453	rVB4	6194	11259	2.90%	0.350%
6	3.815	847	863	889	rBV	32415	122992	31.67%	3.824%
7	4.256	982	1000	1025	rBV3	55171	168033	43.27%	5.224%
8	4.375	1025	1037	1055	rVB3	9644	28303	7.29%	0.880%
9	4.960	1201	1219	1237	rBV3	130003	329523	84.86%	10.244%
10	5.056	1242	1249	1270	rVB6	12936	34638	8.92%	1.077%
11	5.535	1387	1398	1416	rBV2	113817	240095	61.83%	7.464%
12	5.616	1417	1423	1438	rVB2	9614	21893	5.64%	0.681%
13	5.992	1528	1540	1555	rBV2	77598	164913	42.47%	5.127%
14	6.918	1816	1828	1843	rBV2	34623	69469	17.89%	2.160%
15	7.246	1919	1930	1961	rBV	146996	287729	74.09%	8.945%
16	7.561	2018	2028	2049	rBV2	21022	45238	11.65%	1.406%
17	7.879	2117	2127	2138	rBV	5445	9625	2.48%	0.299%
18	8.031	2164	2174	2208	rBV	175562	388328	100.00%	12.073%
19	8.789	2399	2410	2437	rBV	197324	349060	89.89%	10.852%
20	10.156	2824	2835	2852	rBV	64978	107878	27.78%	3.354%
21	10.329	2878	2889	2899	rVB2	11377	18031	4.64%	0.561%
22	11.188	3145	3156	3171	rBV	192828	305968	78.79%	9.512%
23	11.564	3261	3273	3289	rBV	157666	254935	65.65%	7.926%
24	12.198	3461	3470	3476	rBV2	3245	4959	1.28%	0.154%




Sum of corrected areas: 3216609

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032637.D
Acq On : 25 Oct 2023 16:48
Operator : SY/MD
Sample : 04962-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COALO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

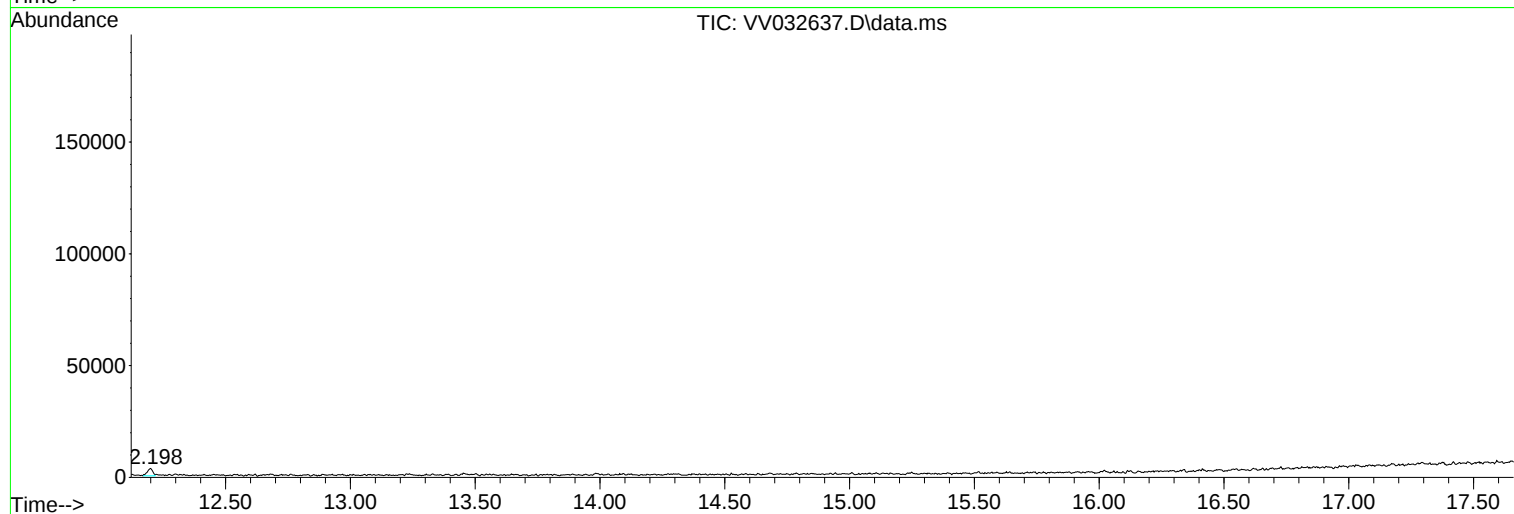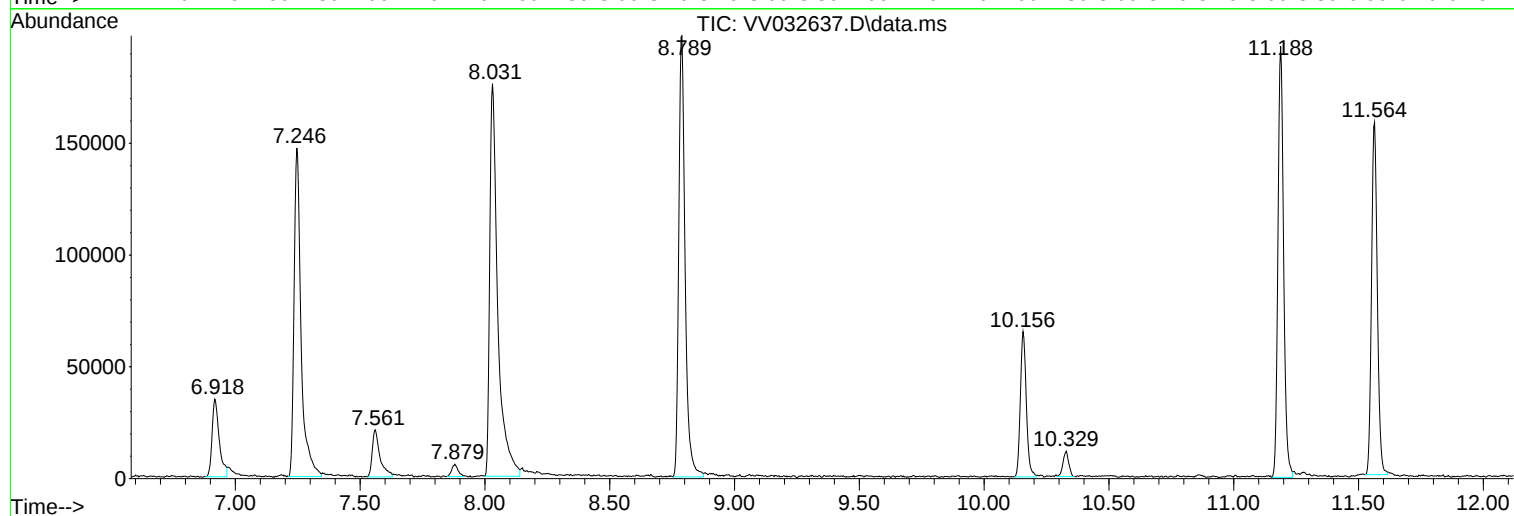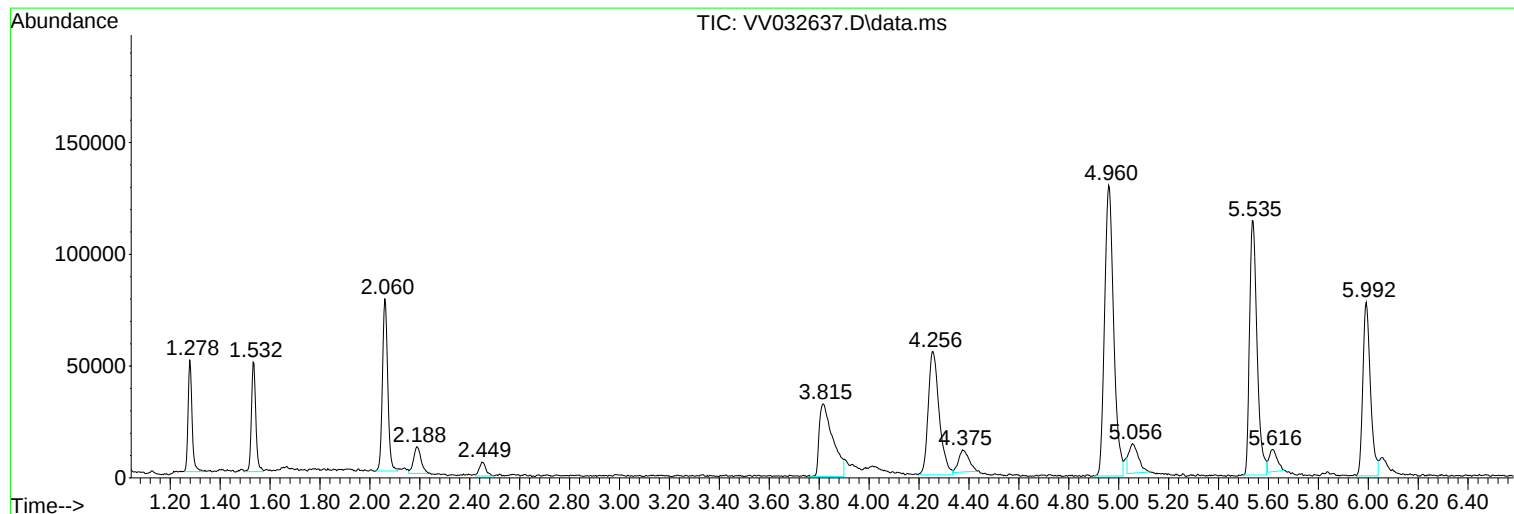

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032637.D
Acq On : 25 Oct 2023 16:48
Operator : SY/MD
Sample : 04962-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032637.D
Acq On : 25 Oct 2023 16:48
Operator : SY/MD
Sample : 04962-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------