

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
 Data File : VV032645.D
 Acq On : 25 Oct 2023 20:02
 Operator : SY/MD
 Sample : 04961-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LJ7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	51851	55428	14.33%	1.848%
2	1.532	146	153	169	rVB	49119	57829	14.95%	1.928%
3	2.060	307	317	333	rBV	80196	117757	30.44%	3.926%
4	2.182	346	355	368	rVB2	11104	20235	5.23%	0.675%
5	2.449	429	438	445	rBV5	3162	5124	1.32%	0.171%
6	3.815	852	863	886	rBV	22985	82283	21.27%	2.743%
7	4.252	984	999	1021	rBV2	54298	145538	37.62%	4.852%
8	4.362	1025	1033	1055	rVB3	8539	25266	6.53%	0.842%
9	4.960	1203	1219	1237	rBV3	129543	333443	86.19%	11.117%
10	5.535	1386	1398	1415	rBV	102381	215032	55.58%	7.169%
11	5.613	1416	1422	1445	rVB3	9974	25876	6.69%	0.863%
12	5.992	1526	1540	1555	rBV2	79642	169529	43.82%	5.652%
13	6.918	1817	1828	1842	rBV2	34183	68731	17.76%	2.291%
14	7.246	1919	1930	1949	rBV	147676	280609	72.53%	9.355%
15	7.558	2019	2027	2046	rBV	21346	42905	11.09%	1.430%
16	8.030	2162	2174	2218	rBV	145609	386892	100.00%	12.899%
17	8.786	2399	2409	2436	rBV	175648	306020	79.10%	10.202%
18	9.082	2491	2501	2509	rBV7	3427	5955	1.54%	0.199%
19	10.156	2825	2835	2856	rBV	65263	109702	28.35%	3.657%
20	10.326	2878	2888	2897	rBV5	3059	4221	1.09%	0.141%
21	11.188	3145	3156	3172	rBV	167125	266949	69.00%	8.900%
22	11.497	3245	3252	3262	rBV	3584	7711	1.99%	0.257%
23	11.564	3262	3273	3287	rVV	156088	251442	64.99%	8.383%
24	12.294	3492	3500	3515	rBV5	8485	15029	3.88%	0.501%




Sum of corrected areas: 2999506

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032645.D
Acq On : 25 Oct 2023 20:02
Operator : SY/MD
Sample : 04961-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LJ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

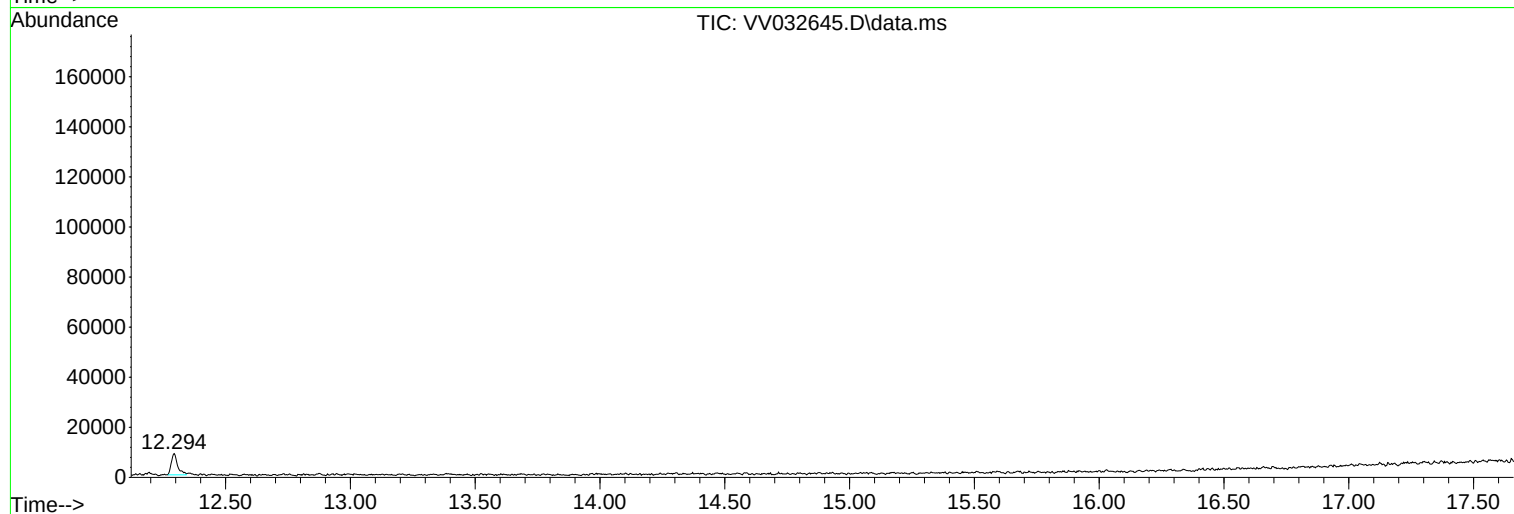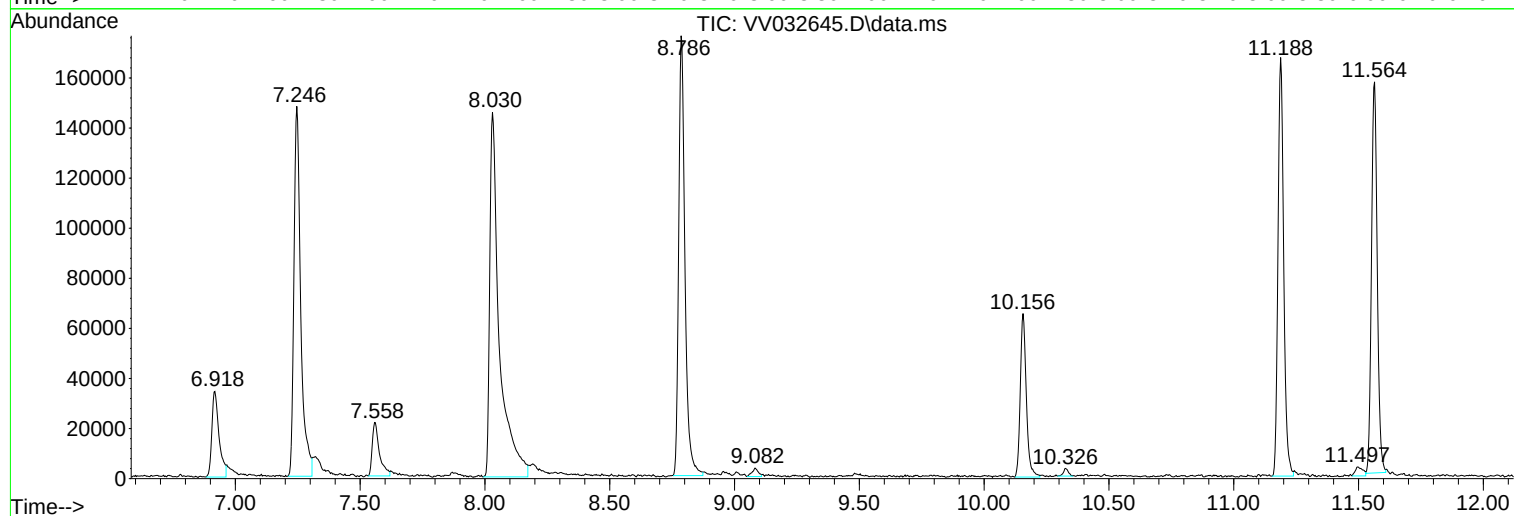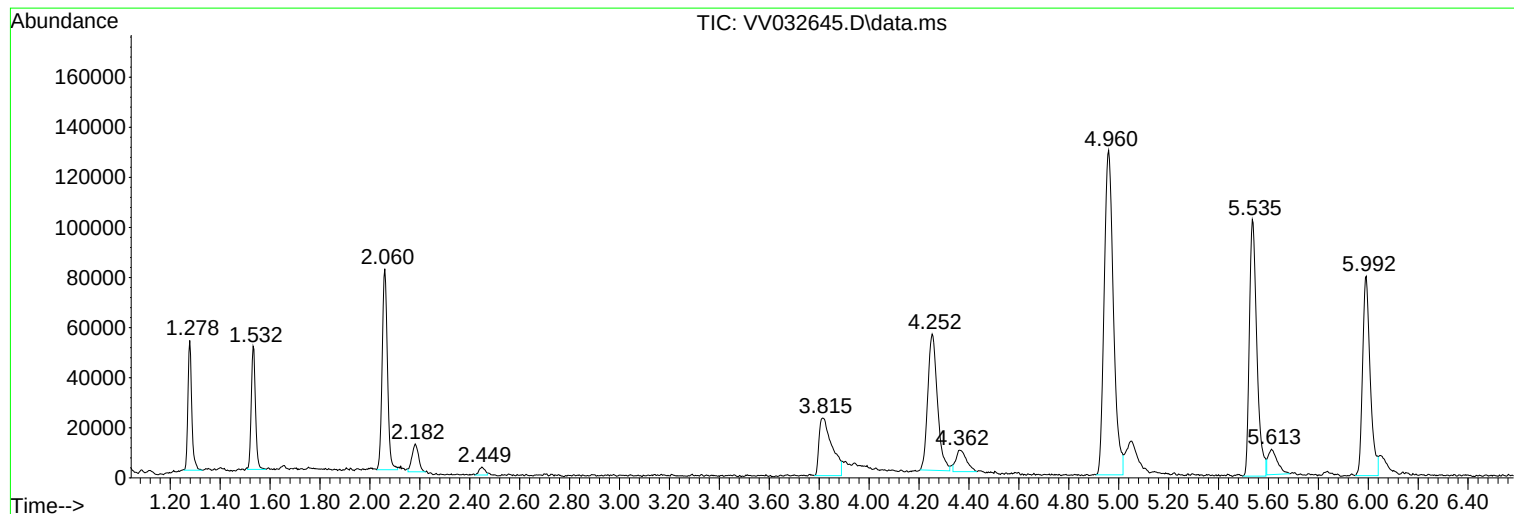

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032645.D
Acq On : 25 Oct 2023 20:02
Operator : SY/MD
Sample : 04961-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LJ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102523\
Data File : VV032645.D
Acq On : 25 Oct 2023 20:02
Operator : SY/MD
Sample : 04961-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LJ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
