

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
 Data File : VV028714.D
 Acq On : 27 Oct 2022 12:48
 Operator : SY/MD
 Sample : N5232-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA90

Quant Time: Oct 28 02:16:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 28 02:13:29 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.616	114	165415	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.847	117	156399	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.243	152	67116	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.304	65	72924	6.339	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	126.800%	
7) Chloroethane-d5		1.565	69	66679	6.855	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	137.000%#	
11) 1,1-Dichloroethene-d2		2.105	63	100833	4.531	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.600%	
20) 2-Butanone-d5		3.889	46	184616	70.377	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	140.760%#	
24) Chloroform-d		4.343	84	116947	5.854	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.000%	
26) 1,2-Dichloroethane-d4		5.031	65	64639	6.377	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	127.600%	
32) Benzene-d6		5.047	84	234760	5.613	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.200%	
36) 1,2-Dichloropropane-d6		6.066	67	83387	6.298	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	126.000%	
41) Toluene-d8		7.314	98	188190	5.766	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.400%	
43) trans-1,3-Dichloroprop...		7.625	79	11937	2.902	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	58.000%	
46) 2-Hexanone-d5		8.088	63	114606	59.854	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	119.700%	
56) 1,1,2,2-Tetrachloroeth...		10.211	84	54334	6.188	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	123.800%#	
66) 1,2-Dichlorobenzene-d4		11.616	152	58345	6.302	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	126.000%#	
Target Compounds							
13) Acetone		2.179	43	9759	6.268	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028714.D
Acq On : 27 Oct 2022 12:48
Operator : SY/MD
Sample : N5232-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA90

Quant Time: Oct 28 02:16:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 28 02:13:29 2022
Response via : Initial Calibration

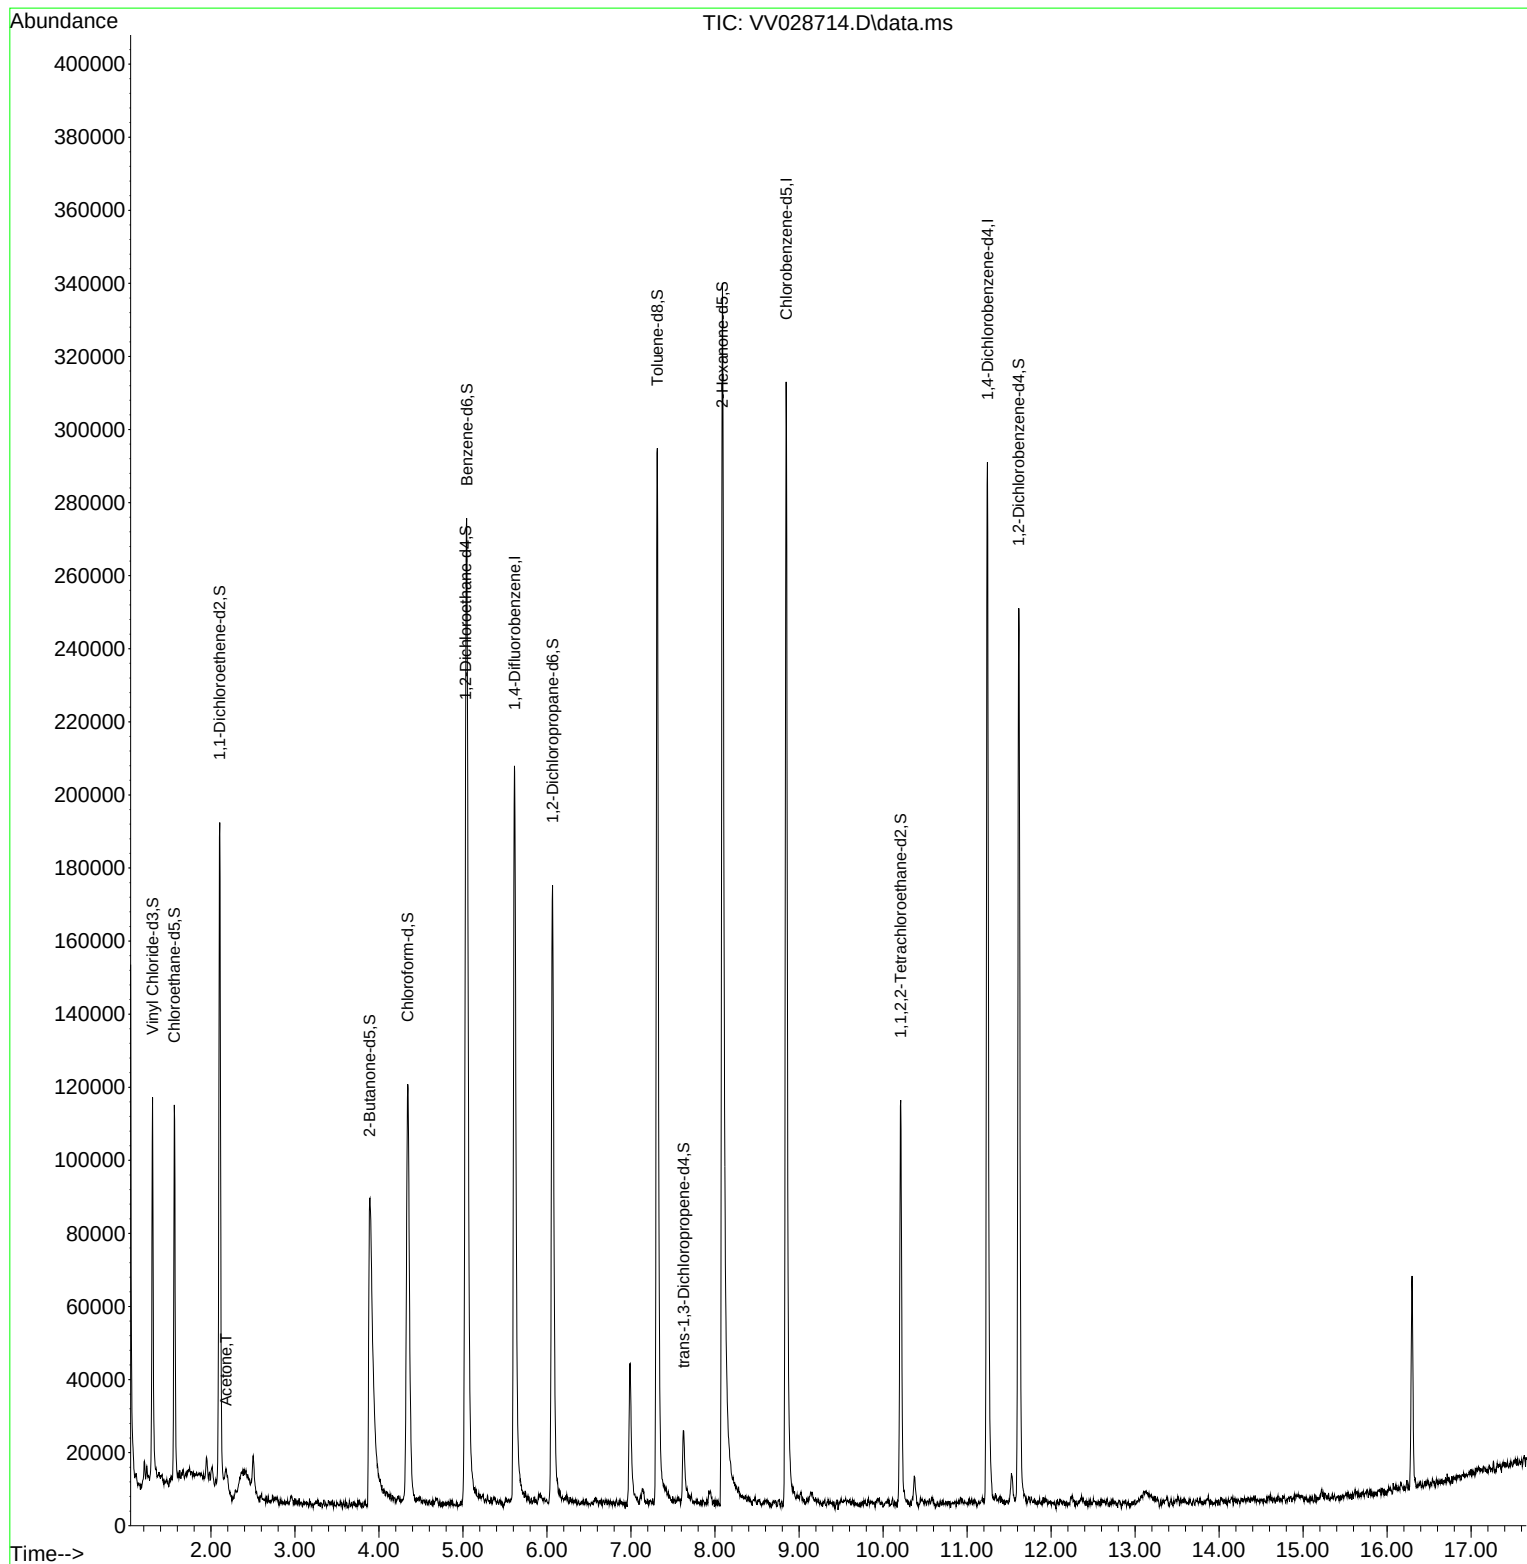

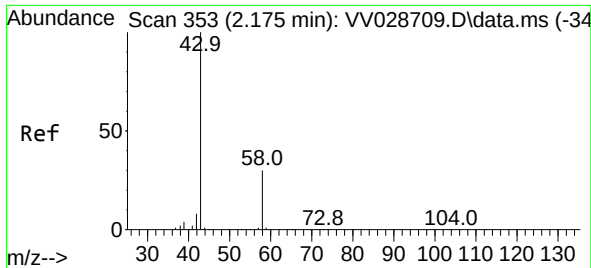

#13

Acetone

Concen: 6.268 ug/L

RT: 2.179 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV028714.D

Acq: 27 Oct 2022 12:48

Instrument :

MSVOA_V

ClientSampleId :

BHA90

Tgt Ion: 43 Resp: 9759

Ion Ratio Lower Upper

43 100

58 29.9 0.0 50.2

