

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102722\
 Data File : VW028725.D
 Acq On : 27 Oct 2022 17:40
 Operator : SY/MD
 Sample : VIBLK303
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK303

Quant Time: Oct 28 02:19:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 28 02:13:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	264987	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	236659	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	107179	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	73515	3.989	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.800%
7) Chloroethane-d5	1.564	69	73588	4.722	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.400%
11) 1,1-Dichloroethene-d2	2.105	63	121232	3.401	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.000%
20) 2-Butanone-d5	3.895	46	185382	44.114	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.220%
24) Chloroform-d	4.342	84	140496	4.390	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
26) 1,2-Dichloroethane-d4	5.027	65	70382	4.334	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
32) Benzene-d6	5.043	84	286015	4.519	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%
36) 1,2-Dichloropropane-d6	6.063	67	97647	4.874	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.400%
41) Toluene-d8	7.310	98	235400	4.767	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.400%
43) trans-1,3-Dichloroprop...	7.622	79	19174	3.080	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	61.600%
46) 2-Hexanone-d5	8.088	63	138116	47.670	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.340%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	59111	4.449	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.000%
66) 1,2-Dichlorobenzene-d4	11.619	152	73896	4.999	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.000%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	13127	0.654	ug/L	89
33) Benzene	5.098	78	43343	0.613	ug/L	100
42) Toluene	7.391	91	28100	0.419	ug/L	99
51) Chlorobenzene	8.882	112	4427	0.105	ug/L	89
52) Ethylbenzene	9.014	91	19262	0.258	ug/L	100
53) m,p-Xylene	9.133	106	22400	0.832	ug/L	87
54) o-Xylene	9.542	106	1875	0.069	ug/L	73
62) 1,3,5-Trimethylbenzene	10.535	105	1887	0.096	ug/L	88
63) 1,2,4-Trimethylbenzene	10.911	105	7168	0.132	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028725.D
Acq On : 27 Oct 2022 17:40
Operator : SY/MD
Sample : VIBLK303
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK303

Quant Time: Oct 28 02:19:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 28 02:13:29 2022
Response via : Initial Calibration




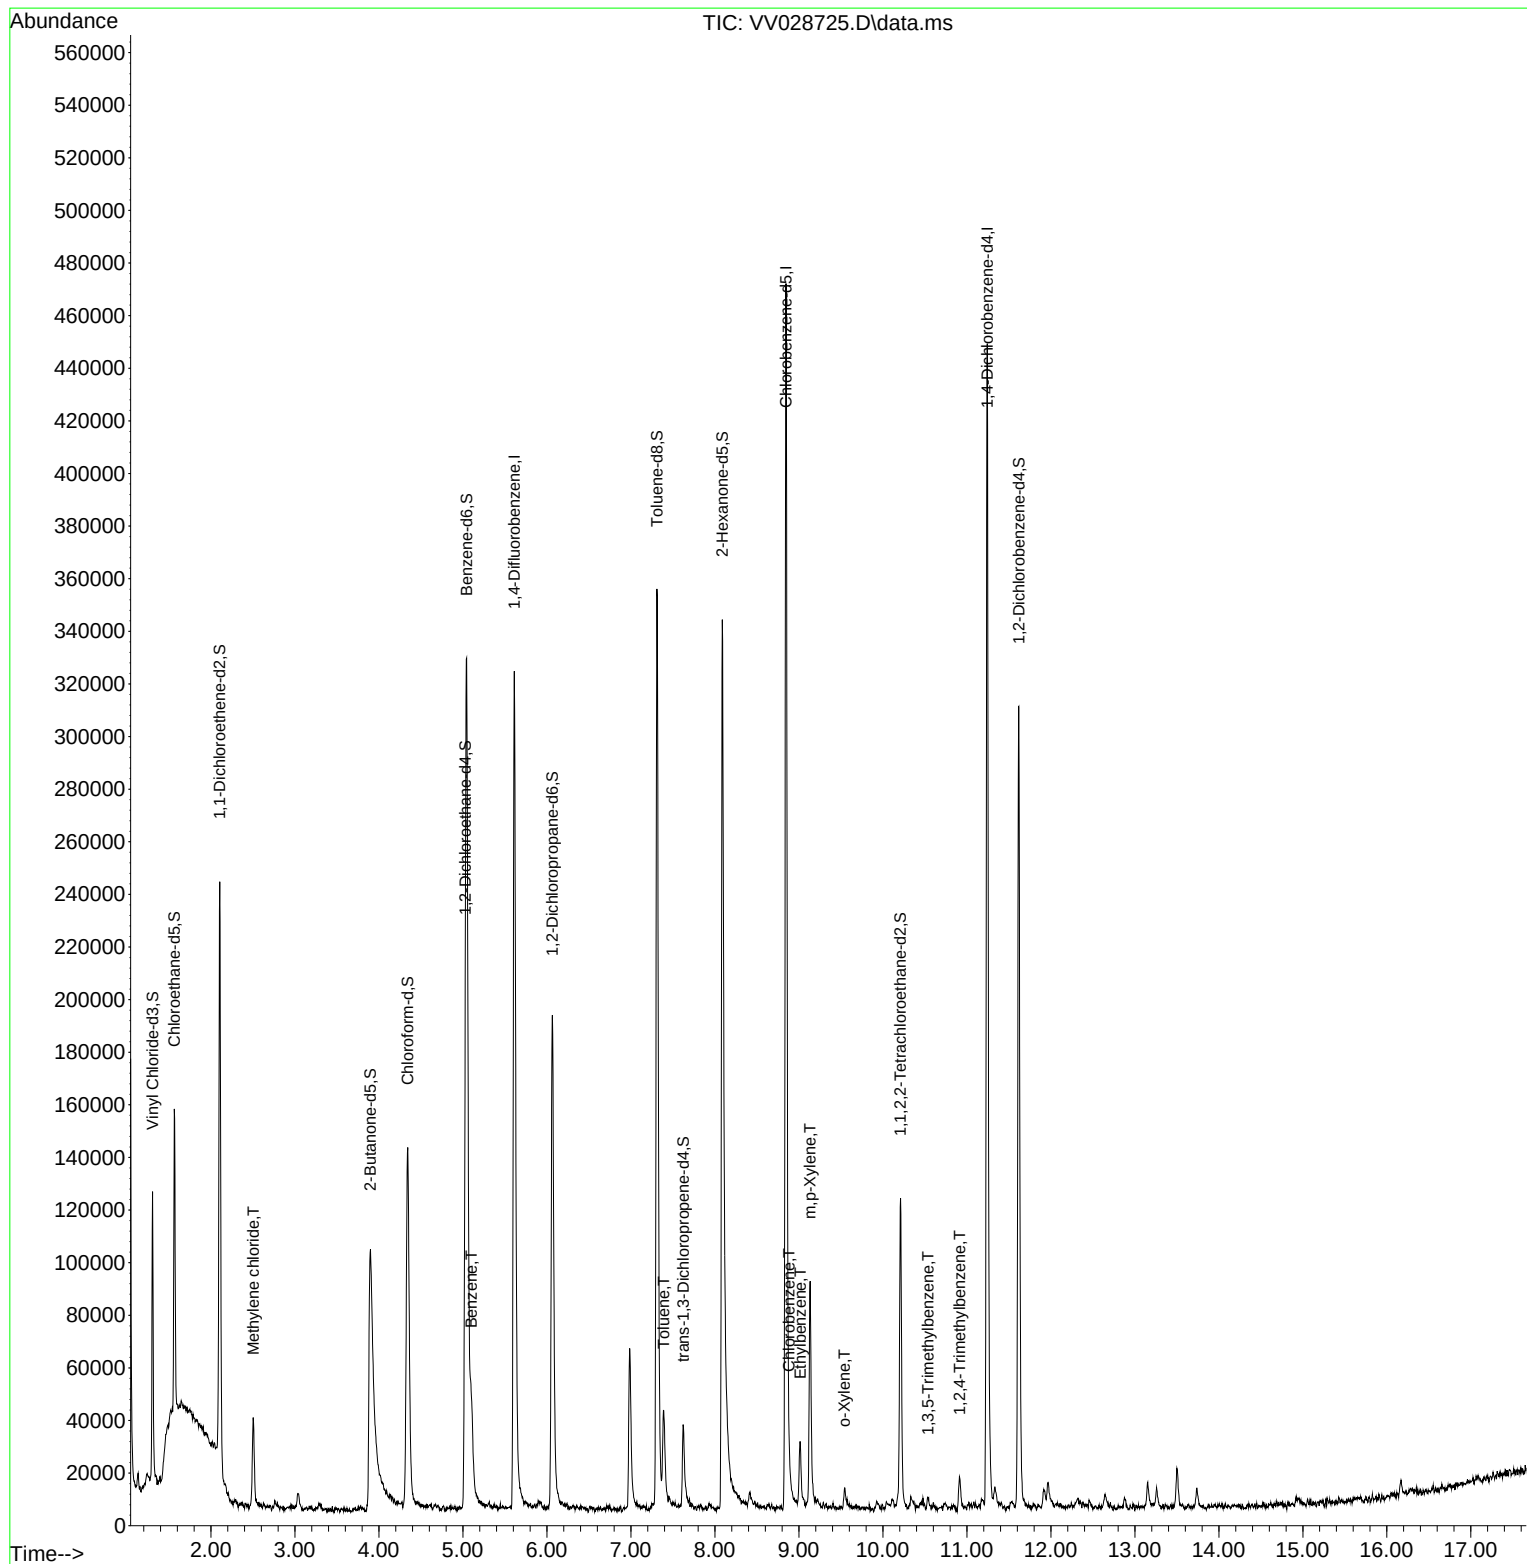


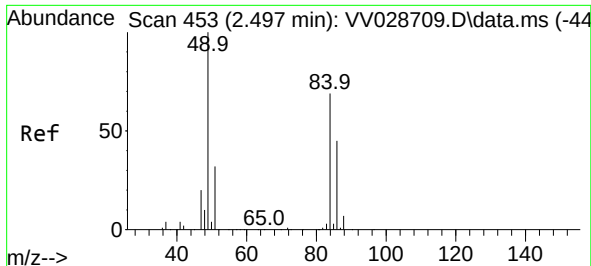

#16
Methylene chloride
Concen: 0.654 ug/L
RT: 2.503 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV028725.D
Acq: 27 Oct 2022 17:40




Instrument :
MSVOA_V
ClientSampleId :
VIBLK303


Tgt Ion: 84 Resp: 13127
Ion Ratio Lower Upper
84 100
86 73.7 44.4 82.4
49 170.9 110.8 205.8

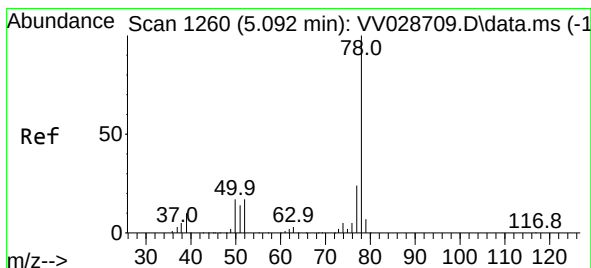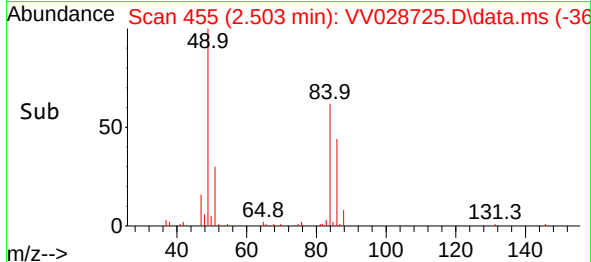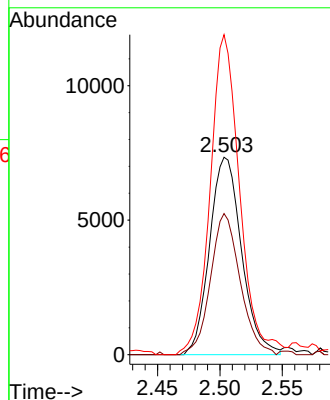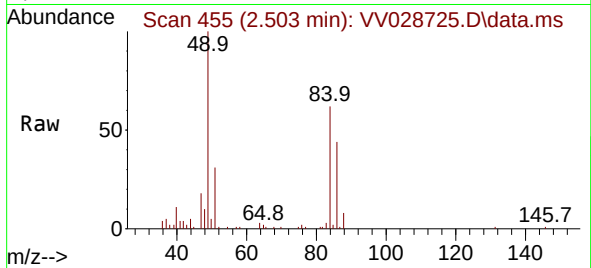

#33
Benzene
Concen: 0.613 ug/L
RT: 5.098 min Scan# 1262
Delta R.T. 0.006 min
Lab File: VV028725.D
Acq: 27 Oct 2022 17:40

Tgt Ion: 78 Resp: 43343

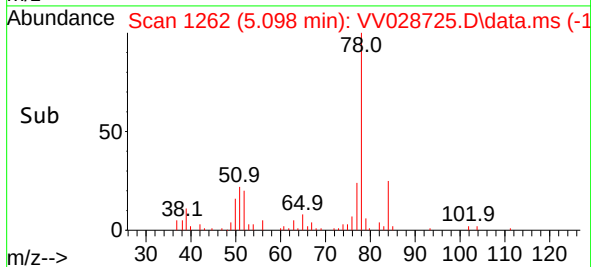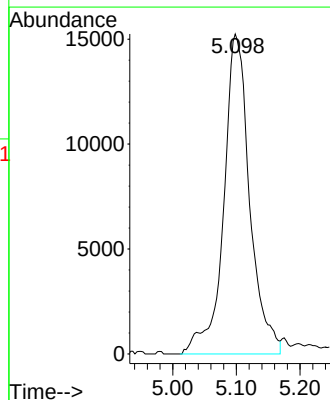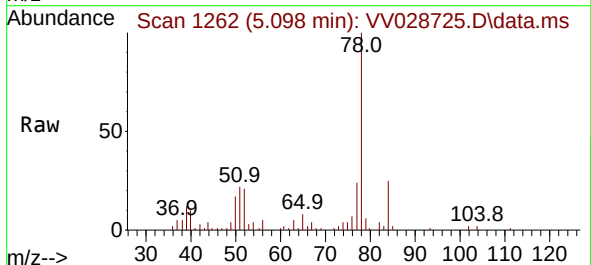

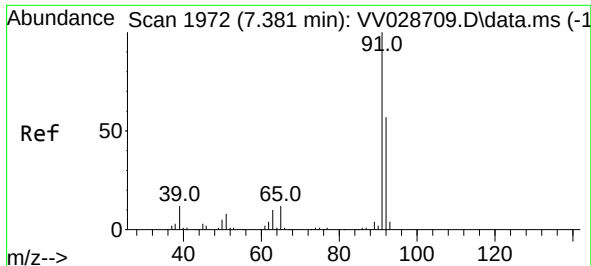

#42

Toluene

Concen: 0.419 ug/L

RT: 7.391 min Scan# 1972

Delta R.T. 0.010 min

Lab File: VV028725.D

Acq: 27 Oct 2022 17:40

Instrument :

MSVOA_V

ClientSampleId :





VIBLK303

Tgt Ion: 91 Resp: 28100

Ion Ratio Lower Upper

91 100

92 58.5 40.5 75.3

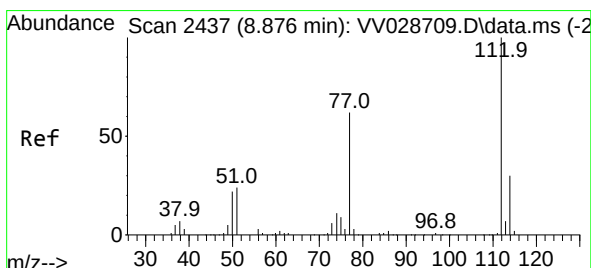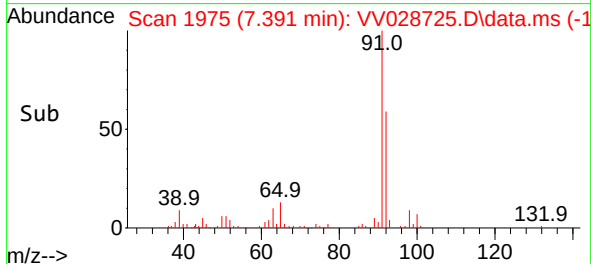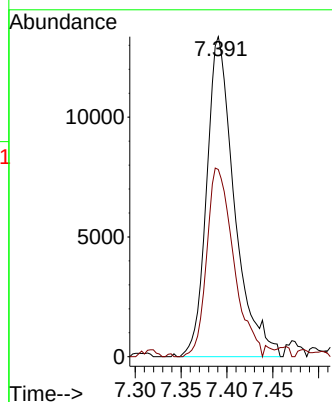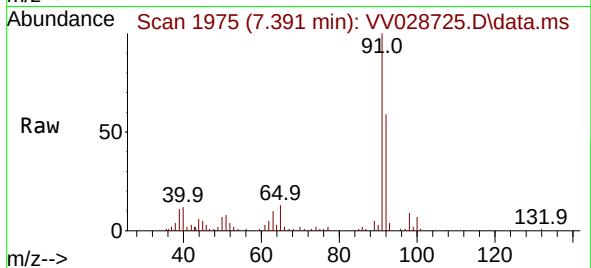

#51

Chlorobenzene

Concen: 0.105 ug/L

RT: 8.882 min Scan# 2439

Delta R.T. 0.006 min

Lab File: VV028725.D

Acq: 27 Oct 2022 17:40




Tgt Ion: 112 Resp: 4427


Ion Ratio Lower Upper

112 100

114 34.4 22.0 41.0

77 72.8 50.0 75.0

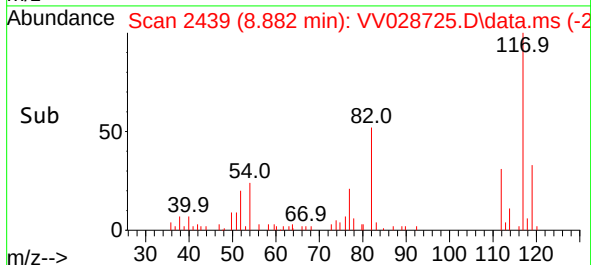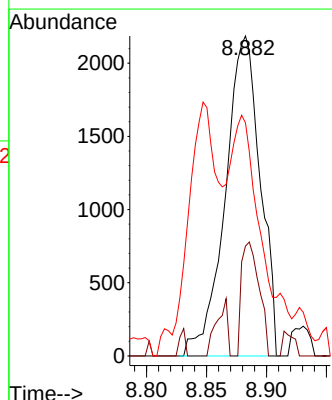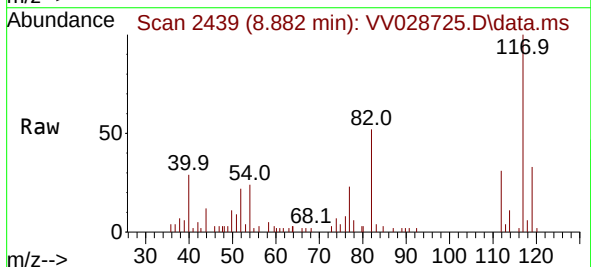

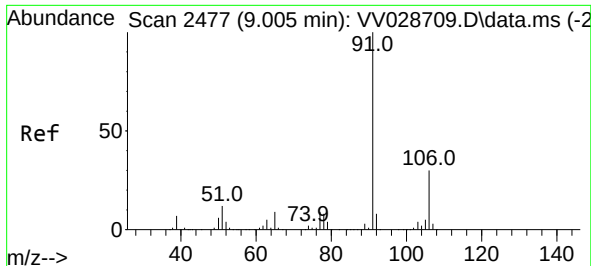

#52

Ethylbenzene

Concen: 0.258 ug/L

RT: 9.014 min Scan# 24

Delta R.T. 0.010 min

Lab File: VV028725.D

Acq: 27 Oct 2022 17:40

Instrument :

MSVOA_V

ClientSampleId :





VIBLK303

Tgt Ion: 91 Resp: 19262

Ion Ratio Lower Upper

91 100

106 30.4 21.3 39.6

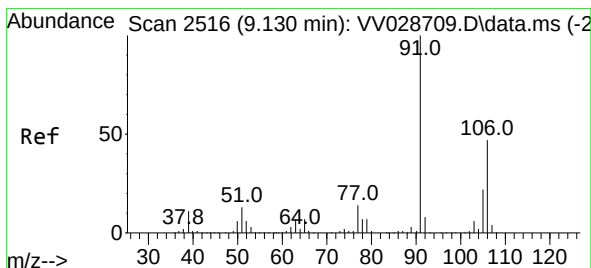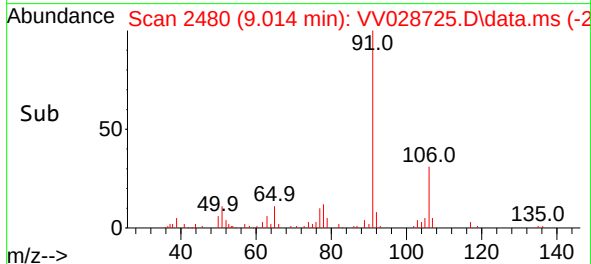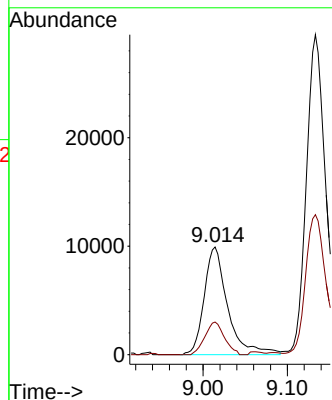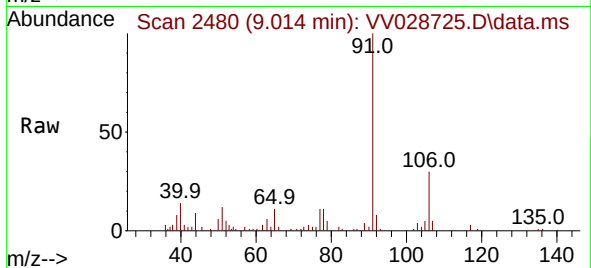

#53

m,p-Xylene

Concen: 0.832 ug/L

RT: 9.133 min Scan# 2517

Delta R.T. 0.003 min

Lab File: VV028725.D




Acq: 27 Oct 2022 17:40


Tgt Ion:106 Resp: 22400

Ion Ratio Lower Upper

106 100

91 228.5 145.5 270.1


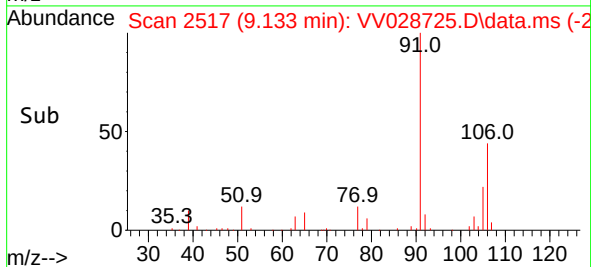
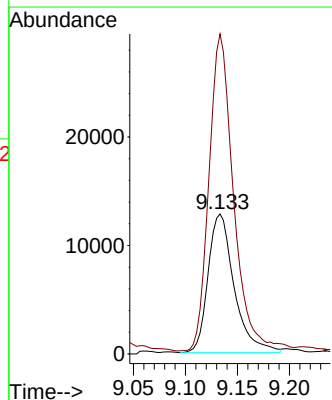
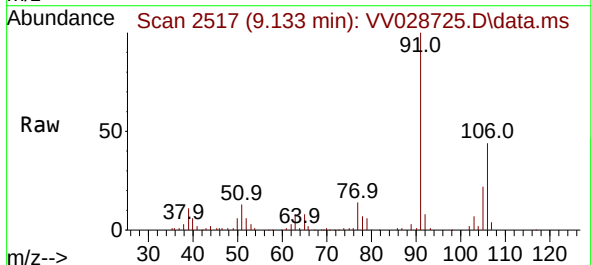


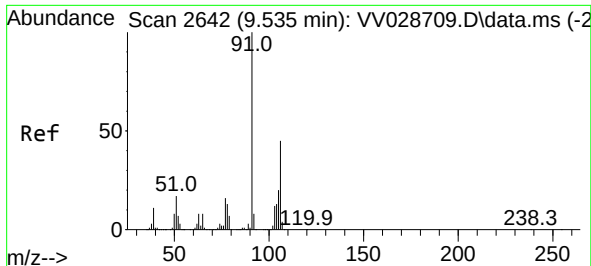

#54
o-Xylene
Concen: 0.069 ug/L
RT: 9.542 min Scan# 2064
Delta R.T. 0.006 min
Lab File: VV028725.D
Acq: 27 Oct 2022 17:40




Instrument :
MSVOA_V
ClientSampleId :
VIBLK303


Tgt Ion:106 Resp: 1875
Ion Ratio Lower Upper
106 100
91 271.5 159.0 295.4

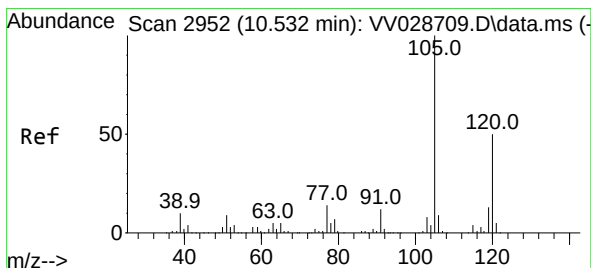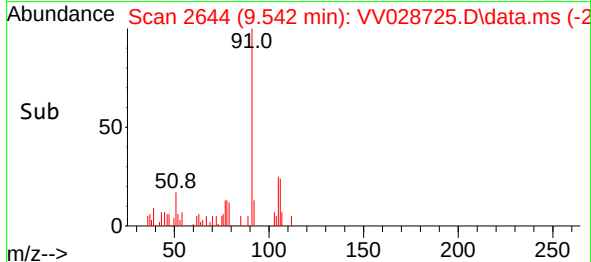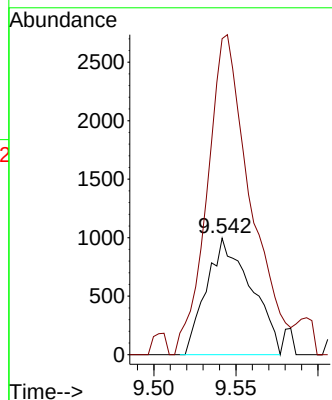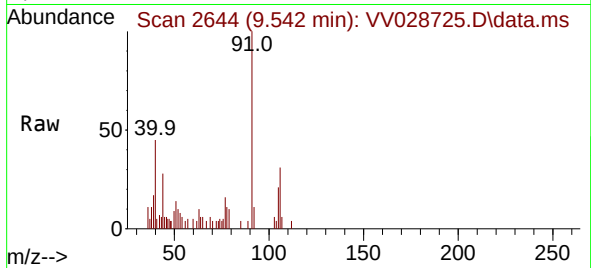

#62
1,3,5-Trimethylbenzene
Concen: 0.096 ug/L
RT: 10.535 min Scan# 2953
Delta R.T. 0.003 min
Lab File: VV028725.D
Acq: 27 Oct 2022 17:40

Tgt Ion:105 Resp: 1887
Ion Ratio Lower Upper
105 100
120 55.8 38.3 57.5

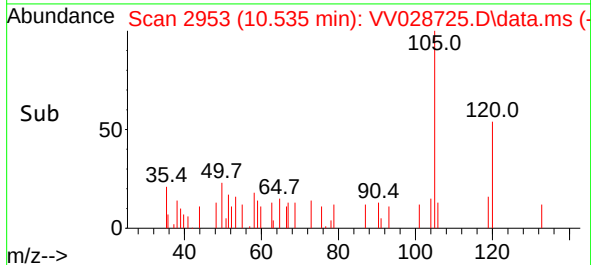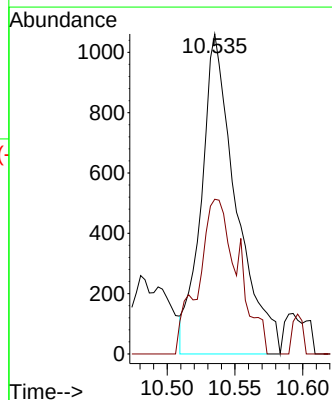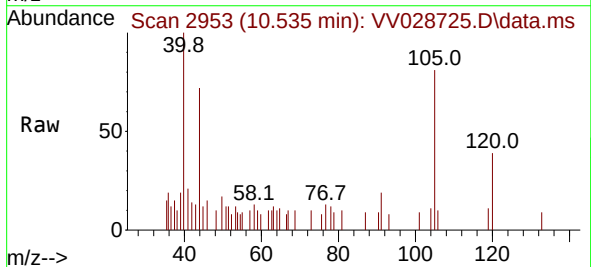

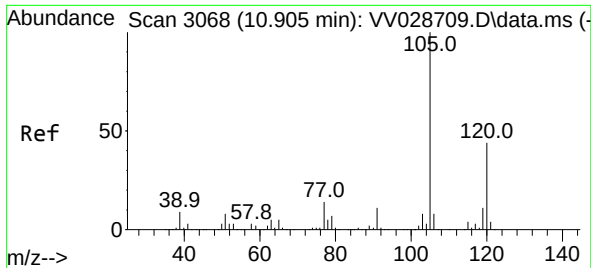

#63
 1,2,4-Trimethylbenzene
 Concen: 0.132 ug/L
 RT: 10.911 min Scan# 3068
 Delta R.T. 0.006 min
 Lab File: VV028725.D
 Acq: 27 Oct 2022 17:40

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK303

Tgt Ion:105 Resp: 7168
 Ion Ratio Lower Upper
 105 100
 120 40.5 36.2 54.2

