

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102722\
 Data File : VW028730.D
 Acq On : 27 Oct 2022 19:43
 Operator : SY/MD
 Sample : N5233-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA76

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 10/28/2022
 Supervised By :Mahesh Dadoda 11/01/2022

Quant Time: Oct 28 02:20:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 28 02:13:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	175650	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	158833	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	70537	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	81979	6.711	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	134.200%#
7) Chloroethane-d5	1.568	69	73636	7.129	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	142.600%#
11) 1,1-Dichloroethene-d2	2.105	63	121632	5.147	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	103.000%
20) 2-Butanone-d5	3.896	46	179633	64.488	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.980%
24) Chloroform-d	4.346	84	131477	6.198	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	124.000%
26) 1,2-Dichloroethane-d4	5.031	65	68997	6.410	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	128.200%
32) Benzene-d6	5.047	84	270713	6.373	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	127.400%#
36) 1,2-Dichloropropane-d6	6.069	67	88385	6.573	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	131.400%
41) Toluene-d8	7.313	98	216477	6.531	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	130.600%#
43) trans-1,3-Dichloroprop...	7.625	79	12000	2.873	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	57.400%
46) 2-Hexanone-d5	8.088	63	116932	60.133	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	120.260%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	57712	6.472	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	129.400%#
66) 1,2-Dichlorobenzene-d4	11.615	152	69391	7.132	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	142.600%#
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.127	85	3728	0.503	ug/L	98
5) Vinyl chloride	1.310	62	151859	11.052	ug/L	97
8) Chloroethane	1.584	64	7601	0.814	ug/L #	59
12) 1,1-Dichloroethene	2.114	96	8806	0.912	ug/L #	1
13) Acetone	2.188	43	13018m	7.874	ug/L	
14) Carbon disulfide	2.291	76	7960	0.357	ug/L #	93
16) Methylene chloride	2.506	84	3952	0.297	ug/L	93
18) trans-1,2-Dichloroethene	2.761	96	6499	0.669	ug/L	86
19) 1,1-Dichloroethane	3.188	63	19508	0.832	ug/L #	94
22) cis-1,2-Dichloroethene	3.902	96	808225	69.390	ug/L #	99
30) Cyclohexane	4.674	56	45828	2.315	ug/L	97
33) Benzene	5.092	78	6967184	146.769	ug/L	100
35) Methylcyclohexane	6.130	83	16078	0.990	ug/L	95
42) Toluene	7.387	91	108217	2.404	ug/L	99
51) Chlorobenzene	8.876	112	697569	24.612	ug/L	98
52) Ethylbenzene	9.008	91	487974	9.755	ug/L	98
53) m,p-Xylene	9.133	106	44150	2.444	ug/L	99
54) o-Xylene	9.538	106	21083	1.160	ug/L	98
60) Isopropylbenzene	9.924	105	140503	3.165	ug/L	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
 Data File : VV028730.D
 Acq On : 27 Oct 2022 19:43
 Operator : SY/MD
 Sample : N5233-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA76


Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 10/28/2022
 Supervised By :Mahesh Dadoda 11/01/2022

Quant Time: Oct 28 02:20:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 28 02:13:29 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
63) 1,2,4-Trimethylbenzene	10.911	105	21413	0.597	ug/L	98
65) 1,4-Dichlorobenzene	11.268	146	29696	1.557	ug/L	97
67) 1,2-Dichlorobenzene	11.635	146	16301	0.932	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

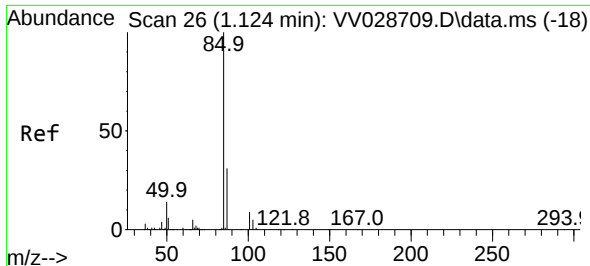

#2
Dichlorodifluoromethane
Concen: 0.503 ug/L
RT: 1.127 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43




Instrument :
MSVOA_V
ClientSampleId :
BHA76

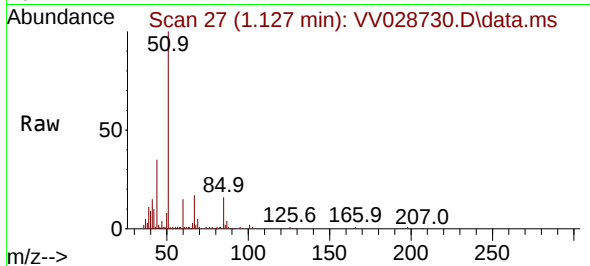


Tgt Ion: 85 Resp: 3728
Ion Ratio Lower Upper
85 100
87 34.6 26.6 40.0

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 10/28/2022
Supervised By :Mahesh Dadoda 11/01/2022

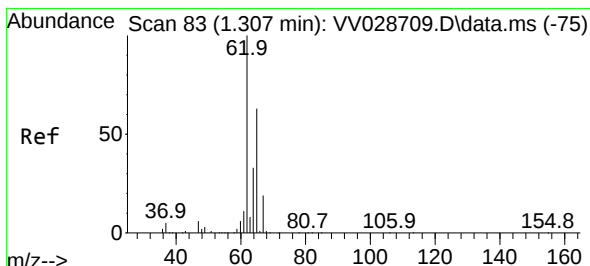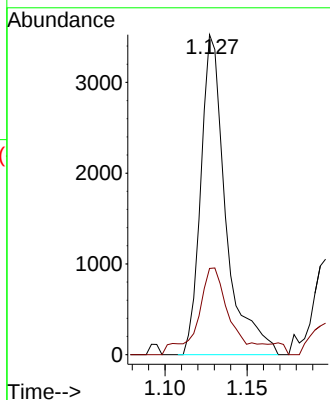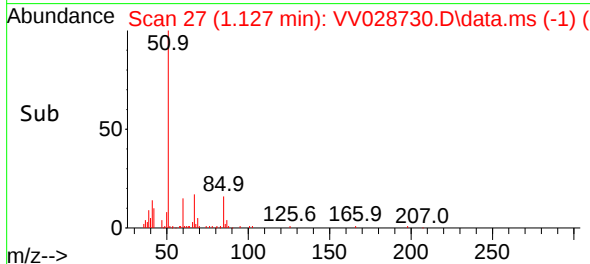


#5
Vinyl chloride
Concen: 11.052 ug/L
RT: 1.310 min Scan# 84
Delta R.T. 0.003 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43

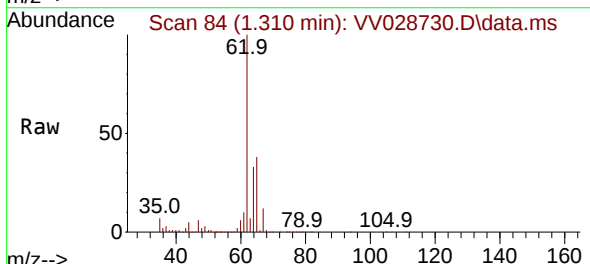


Tgt Ion: 62 Resp: 151859
Ion Ratio Lower Upper
62 100
64 32.9 22.0 41.0

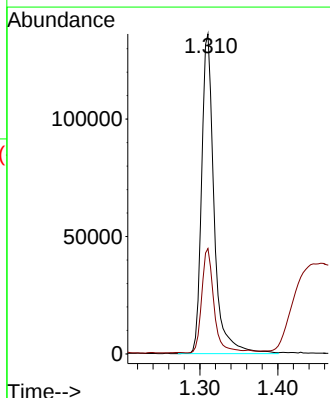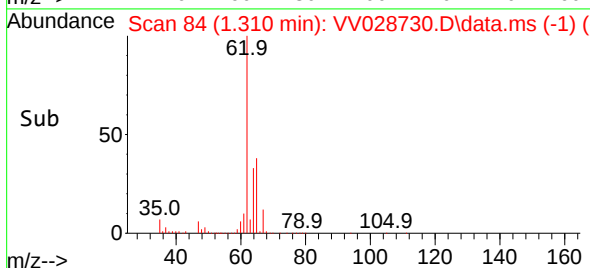



#8
Chloroethane
Concen: 0.814 ug/L
RT: 1.584 min Scan# 168
Delta R.T. 0.003 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43




Instrument :
MSVOA_V
ClientSampleId :
BHA76



Tgt Ion: 64 Resp: 760
Ion Ratio Lower Upper
64 100
66 10.4 23.9 44.5




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 10/28/2022
Supervised By :Mahesh Dadoda 11/01/2022

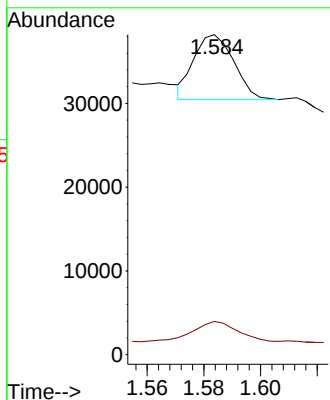

#12
1,1-Dichloroethene
Concen: 0.912 ug/L
RT: 2.114 min Scan# 334
Delta R.T. 0.003 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43


Tgt Ion: 96 Resp: 8806
Ion Ratio Lower Upper
96 100
61 270.7 148.1 275.1
63 874.2 133.3 247.7#

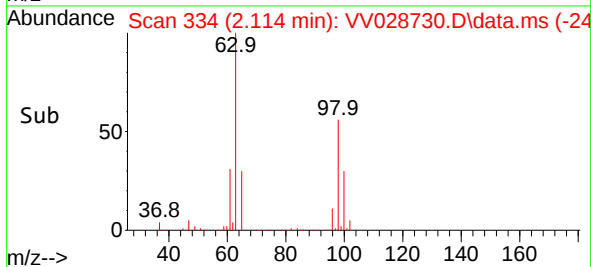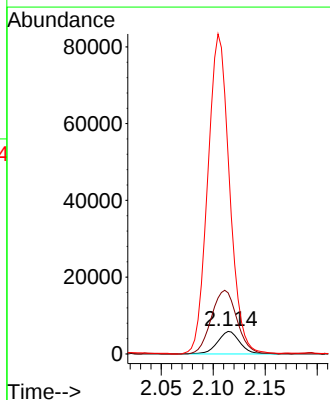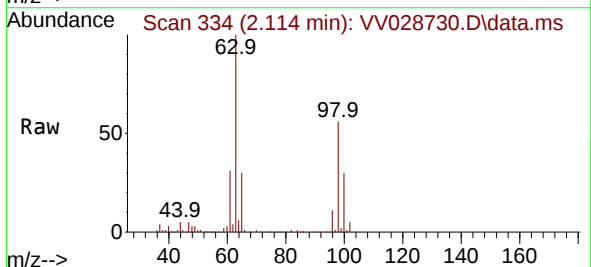



#13
Acetone
Concen: 7.874 ug/L m
RT: 2.188 min Scan# 357
Delta R.T. 0.013 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43




Instrument :
MSVOA_V
ClientSampleId :
BHA76




Tgt Ion: 43 Resp: 13018
Ion Ratio Lower Upper
43 100
58 14.6 0.0 50.2

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 10/28/2022
Supervised By :Mahesh Dadoda 11/01/2022

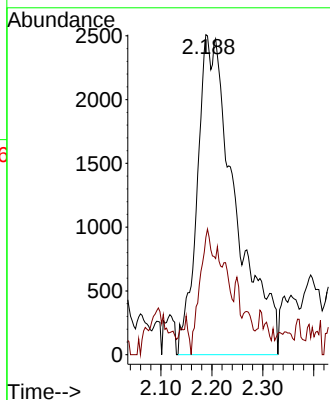


#14
Carbon disulfide
Concen: 0.357 ug/L
RT: 2.291 min Scan# 389
Delta R.T. 0.006 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43

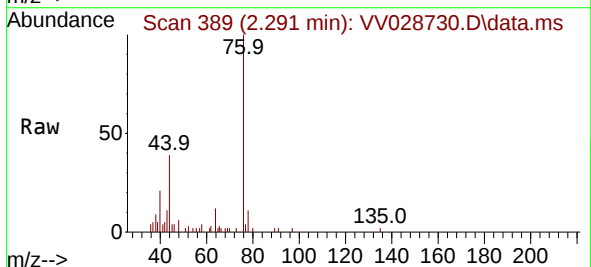


Tgt Ion: 76 Resp: 7960
Ion Ratio Lower Upper
76 100
78 11.4 7.1 10.7#

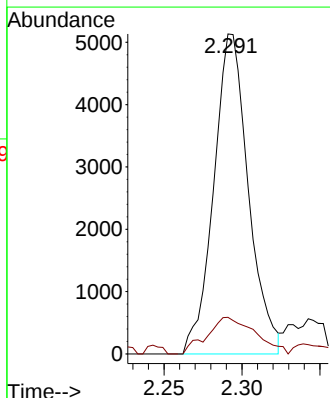



#16
Methylene chloride
Concen: 0.297 ug/L
RT: 2.506 min Scan# 456
Delta R.T. 0.010 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43




Instrument :
MSVOA_V
ClientSampleId :
BHA76



Tgt Ion: 84 Resp: 3952
Ion Ratio Lower Upper
84 100
86 67.1 44.4 82.4
49 148.2 110.8 205.8




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 10/28/2022
Supervised By :Mahesh Dadoda 11/01/2022

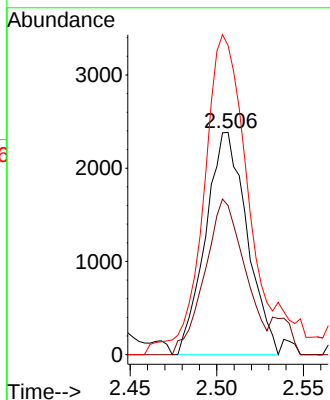

#18
trans-1,2-Dichloroethene
Concen: 0.669 ug/L
RT: 2.761 min Scan# 535
Delta R.T. 0.010 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43


Tgt Ion: 96 Resp: 6499
Ion Ratio Lower Upper
96 100
61 145.1 114.3 212.3
98 51.3 45.0 83.6

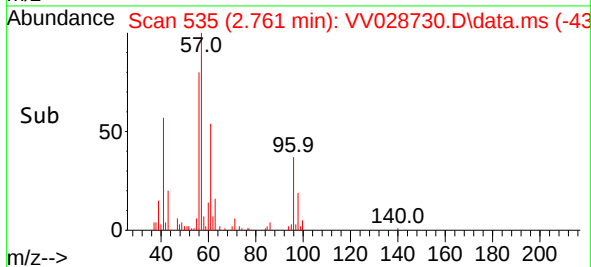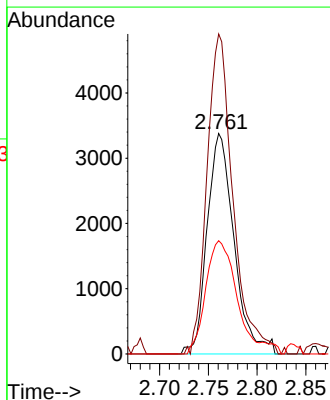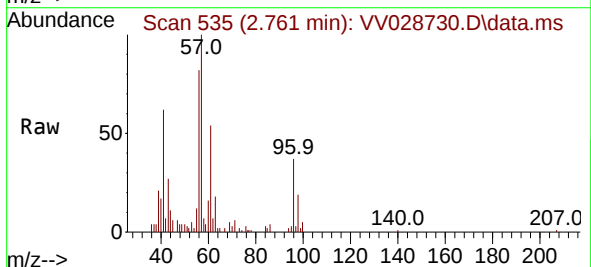



#19
1,1-Dichloroethane
Concen: 0.832 ug/L
RT: 3.188 min Scan# 60
Delta R.T. 0.006 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43




Instrument :
MSVOA_V
ClientSampleId :
BHA76



Tgt Ion: 63 Resp: 19508
Ion Ratio Lower Upper
63 100
65 35.7 23.1 42.9
83 14.9 7.9 14.7




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 10/28/2022
Supervised By :Mahesh Dadoda 11/01/2022

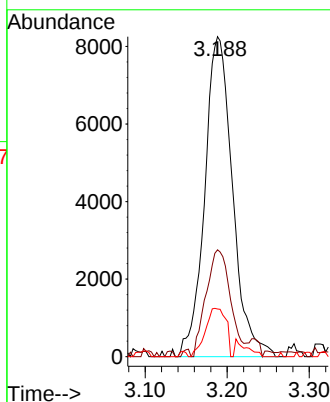

#22
cis-1,2-Dichloroethene
Concen: 69.390 ug/L
RT: 3.902 min Scan# 890
Delta R.T. -0.000 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43

Tgt Ion: 96 Resp: 808225
Ion Ratio Lower Upper
96 100
61 146.3 101.4 188.2
68 0.0 0.5 0.9

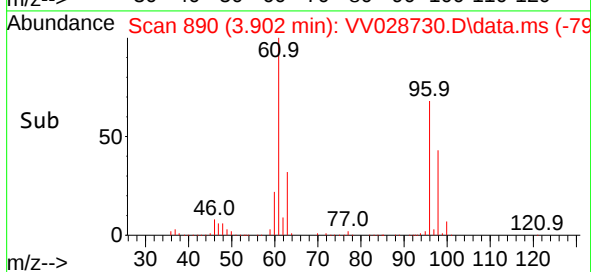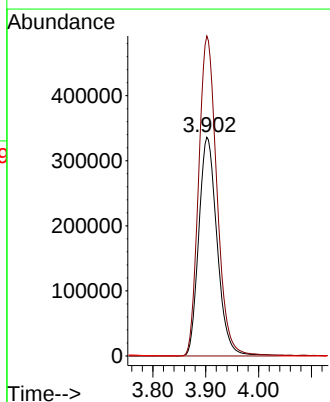



#30

Cyclohexane

Concen: 2.315 ug/L

RT: 4.674 min Scan# 1128

Delta R.T. 0.006 min

Lab File: VV028730.D

Acq: 27 Oct 2022 19:43

Instrument :

MSVOA_V

ClientSampleId :

BHA76

Tgt Ion: 56 Resp: 45828





Ion	Ratio	Lower	Upper
56	100		
69	28.6	22.6	34.0
84	79.3	60.4	90.6

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 10/28/2022

Supervised By :Mahesh Dadoda 11/01/2022

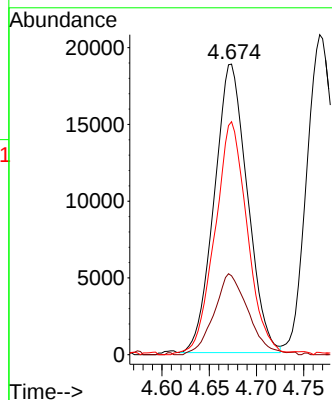

#33

Benzene

Concen: 146.769 ug/L




RT: 5.092 min Scan# 1260


Delta R.T. -0.000 min

Lab File: VV028730.D

Acq: 27 Oct 2022 19:43


Tgt Ion: 78 Resp: 6967184

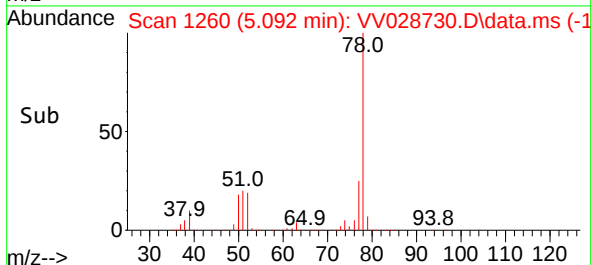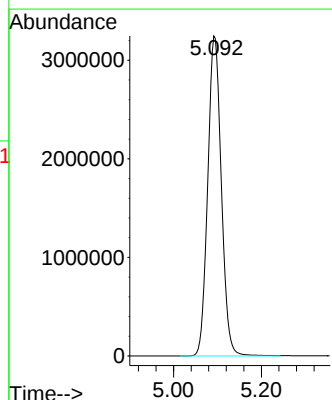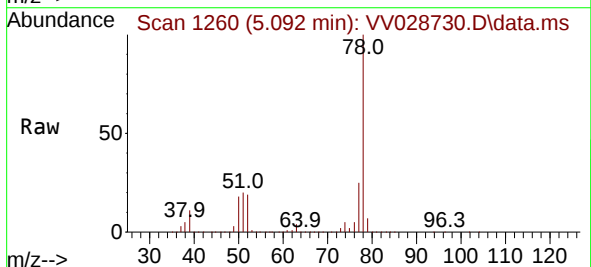



#35
Methylcyclohexane
Concen: 0.990 ug/L
RT: 6.130 min Scan# 1581
Delta R.T. 0.006 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43




Instrument :
MSVOA_V
ClientSampleId :
BHA76



Tgt Ion: 83 Resp: 16078
Ion Ratio Lower Upper
83 100
55 90.4 70.0 105.0
98 49.6 35.6 53.4




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 10/28/2022
Supervised By :Mahesh Dadoda 11/01/2022

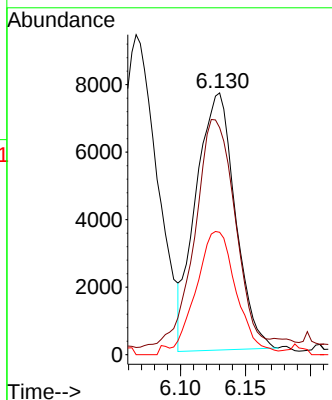

#42
Toluene
Concen: 2.404 ug/L
RT: 7.387 min Scan# 1974
Delta R.T. 0.006 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43

Tgt Ion: 91 Resp: 108217
Ion Ratio Lower Upper
91 100
92 57.4 40.5 75.3

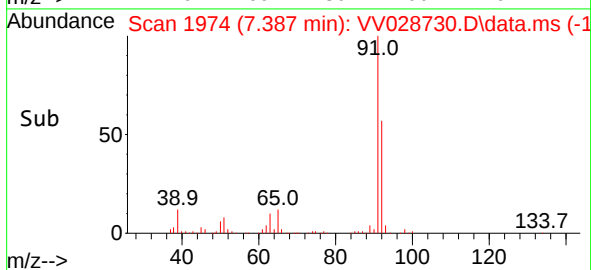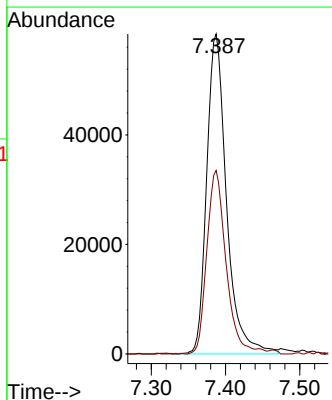







#51
Chlorobenzene
Concen: 24.612 ug/L
RT: 8.876 min Scan# 2437
Delta R.T. -0.000 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43

Instrument :
MSVOA_V
ClientSampleId :
BHA76

Tgt Ion:112 Resp: 697569
Ion Ratio Lower Upper
112 100
114 31.4 22.0 41.0
77 64.8 50.0 75.0




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 10/28/2022
Supervised By :Mahesh Dadoda 11/01/2022

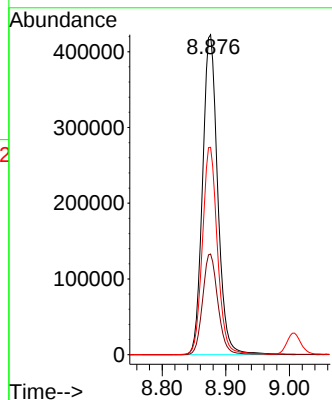

#52
Ethylbenzene
Concen: 9.755 ug/L
RT: 9.008 min Scan# 2478
Delta R.T. 0.003 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43

Tgt Ion: 91 Resp: 487974
Ion Ratio Lower Upper
91 100
106 29.5 21.3 39.6

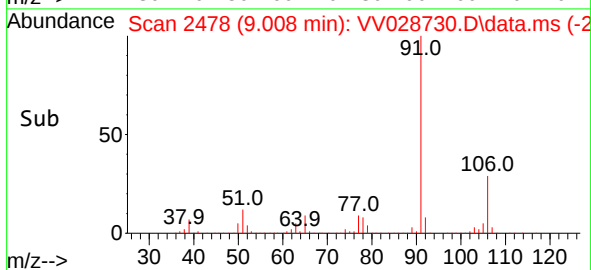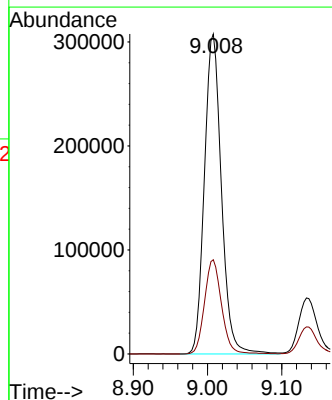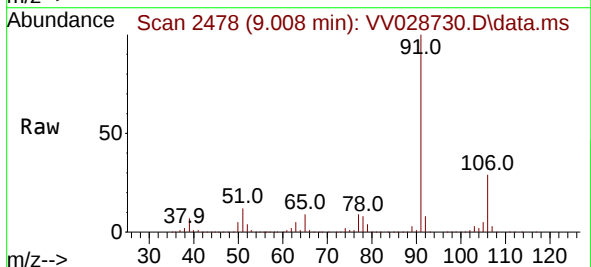







#53
m,p-Xylene
Concen: 2.444 ug/L
RT: 9.133 min Scan# 2516
Delta R.T. 0.003 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43

Instrument :
MSVOA_V
ClientSampleId :
BHA76

Tgt Ion:106 Resp: 44150
Ion Ratio Lower Upper
106 100
91 207.0 145.5 270.1




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 10/28/2022
Supervised By :Mahesh Dadoda 11/01/2022

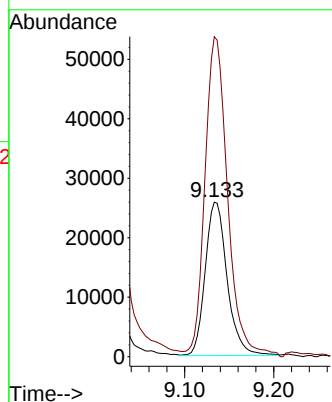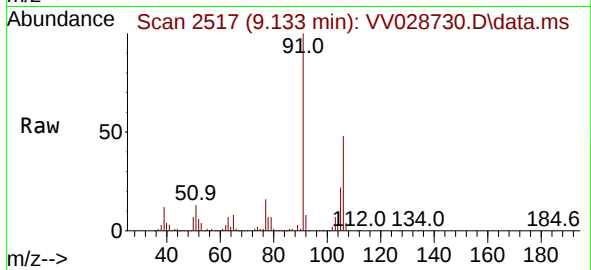

#54
o-Xylene
Concen: 1.160 ug/L
RT: 9.538 min Scan# 2643
Delta R.T. 0.003 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43


Tgt Ion:106 Resp: 21083
Ion Ratio Lower Upper
106 100
91 230.3 159.0 295.4

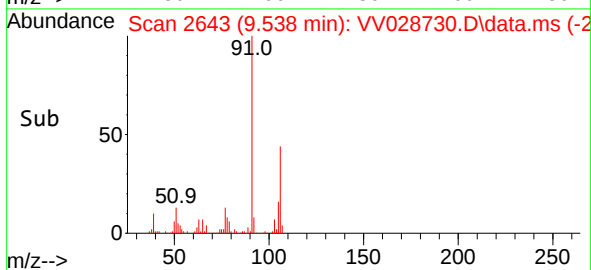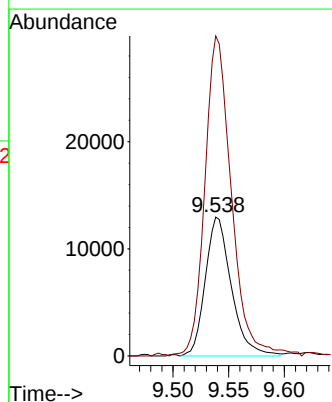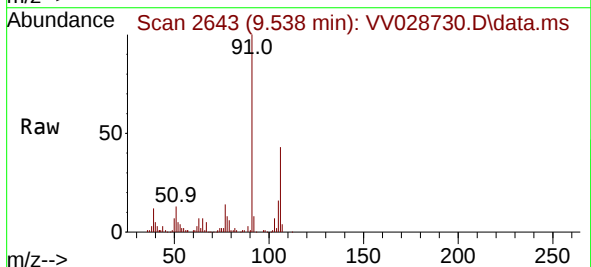



#60
Isopropylbenzene
Concen: 3.165 ug/L
RT: 9.924 min Scan# 21
Delta R.T. -0.000 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43




Instrument :
MSVOA_V
ClientSampleId :
BHA76




Tgt Ion:105 Resp: 14050
Ion Ratio Lower Upper
105 100
120 25.0 20.1 30.1
77 16.9 13.4 20.0

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 10/28/2022
Supervised By :Mahesh Dadoda 11/01/2022

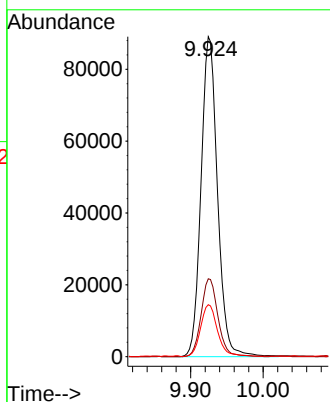


#63
1,2,4-Trimethylbenzene
Concen: 0.597 ug/L
RT: 10.911 min Scan# 3070
Delta R.T. 0.006 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43




Tgt Ion:105 Resp: 21413
Ion Ratio Lower Upper
105 100
120 46.7 36.2 54.2

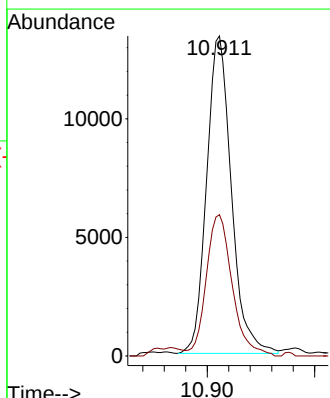



#65
1,4-Dichlorobenzene
Concen: 1.557 ug/L
RT: 11.268 min Scan# 3180
Delta R.T. 0.003 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43




Instrument :
MSVOA_V
ClientSampleId :
BHA76




Tgt Ion:146 Resp: 29690
Ion Ratio Lower Upper
146 100
111 41.9 28.6 53.2
148 60.4 44.3 82.3

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/28/2022
Supervised By :Mahesh Dadoda 11/01/2022

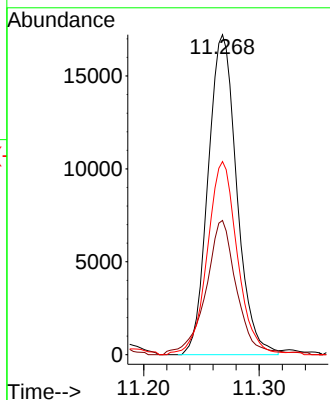

#67
1,2-Dichlorobenzene
Concen: 0.932 ug/L
RT: 11.635 min Scan# 3295
Delta R.T. -0.000 min
Lab File: VV028730.D
Acq: 27 Oct 2022 19:43

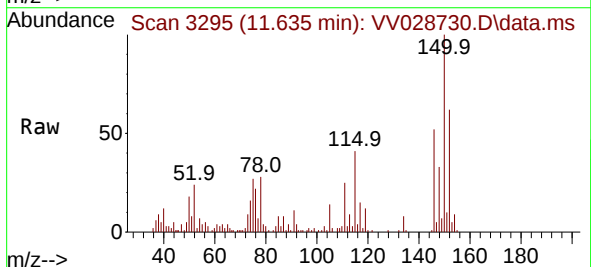

Tgt Ion:146 Resp: 16301
Ion Ratio Lower Upper
146 100
111 48.4 36.2 54.4
148 64.3 50.6 75.8

