

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
 Data File : VV028719.D
 Acq On : 27 Oct 2022 14:49
 Operator : SY/MD
 Sample : N5232-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAB7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028719.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	79192	84697	13.14%	1.545%
2	1.564	155	163	175	rBV	83189	95846	14.87%	1.749%
3	2.105	320	331	346	rVB	152711	224759	34.87%	4.100%
4	2.182	348	355	360	rBV2	4134	6479	1.01%	0.118%
5	3.899	875	889	927	rBV3	52267	223268	34.64%	4.073%
6	4.349	1013	1029	1051	rBV4	114272	361299	56.05%	6.591%
7	5.043	1231	1245	1270	rBV2	237604	595044	92.32%	10.855%
8	5.613	1411	1422	1443	rBV	250599	516687	80.16%	9.426%
9	6.066	1549	1563	1583	rBV	145892	304125	47.18%	5.548%
10	6.985	1838	1849	1867	rBV2	47374	97724	15.16%	1.783%
11	7.133	1886	1895	1906	rBV7	8207	16169	2.51%	0.295%
12	7.313	1939	1951	1969	rBV	255822	460838	71.50%	8.407%
13	7.394	1969	1976	1989	rVB	12522	27342	4.24%	0.499%
14	7.622	2038	2047	2066	rBV	25193	49734	7.72%	0.907%
15	8.091	2183	2193	2233	rBV	246209	622074	96.51%	11.348%
16	8.847	2416	2428	2450	rBV	378464	644565	100.00%	11.759%
17	9.140	2510	2519	2527	rBV7	5599	10759	1.67%	0.196%
18	10.210	2840	2852	2866	rBV2	94712	157559	24.44%	2.874%
19	10.371	2895	2902	2906	rBV10	6303	7870	1.22%	0.144%
20	11.243	3161	3173	3195	rBV	356099	571233	88.62%	10.421%
21	11.615	3278	3289	3307	rBV	228480	378382	58.70%	6.903%
22	12.345	3505	3516	3525	rBV	13750	25119	3.90%	0.458%




Sum of corrected areas: 5481572

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028719.D
Acq On : 27 Oct 2022 14:49
Operator : SY/MD
Sample : N5232-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

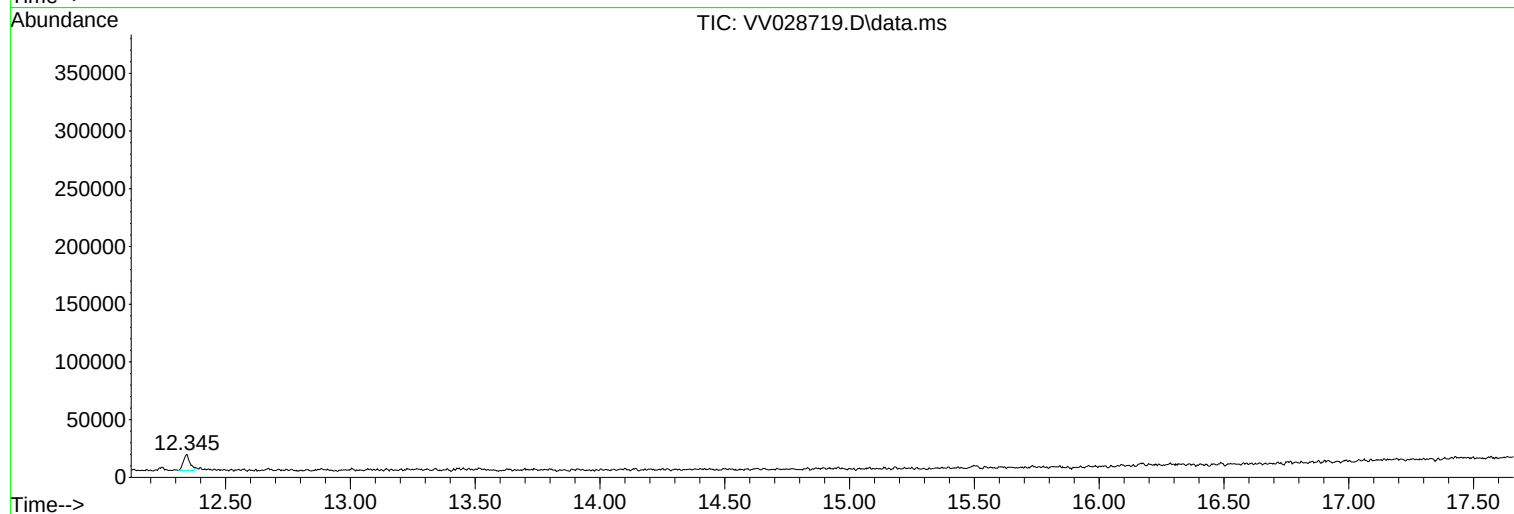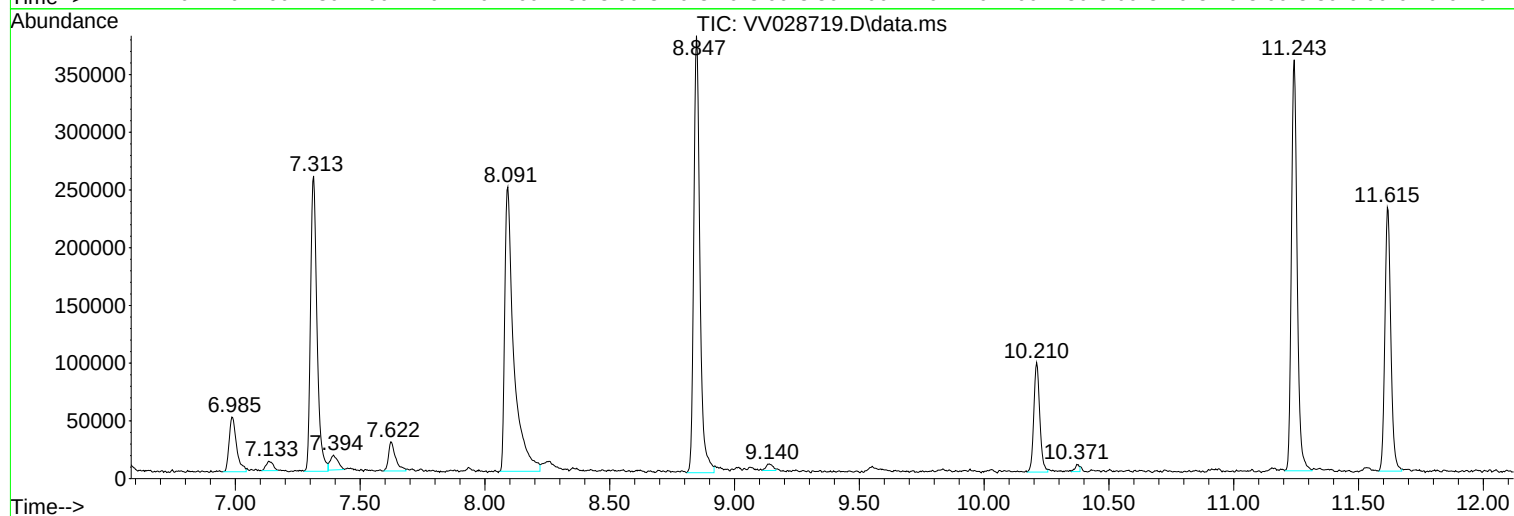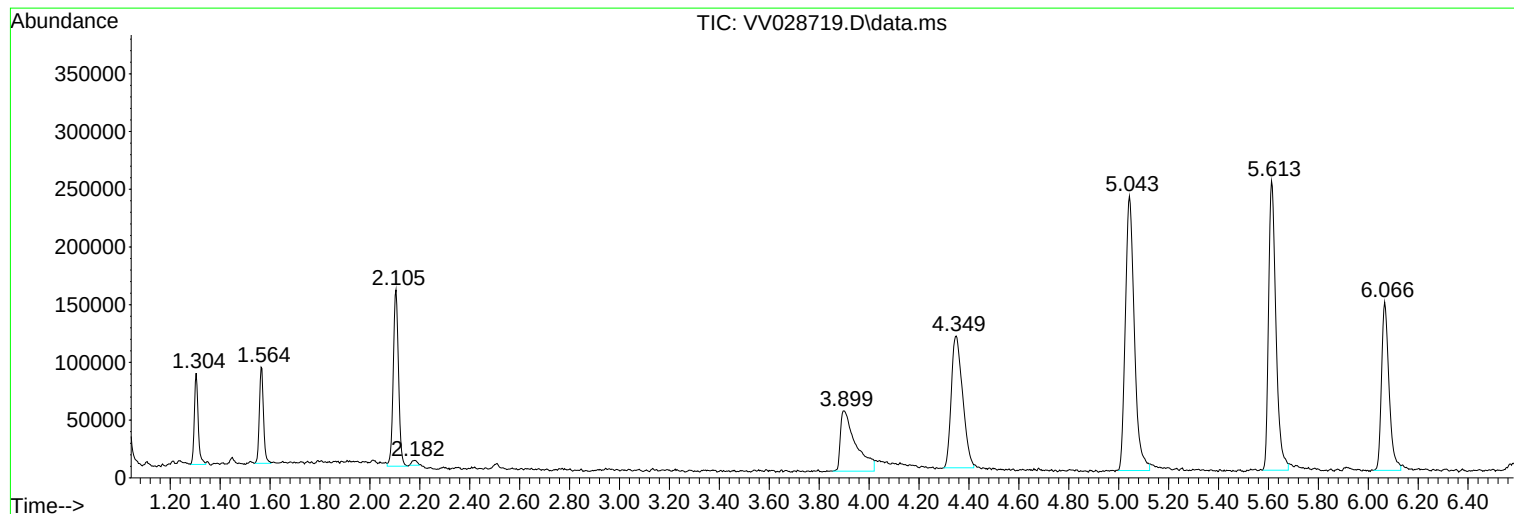

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028719.D
Acq On : 27 Oct 2022 14:49
Operator : SY/MD
Sample : N5232-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028719.D
Acq On : 27 Oct 2022 14:49
Operator : SY/MD
Sample : N5232-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
