

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
 Data File : VV028721.D
 Acq On : 27 Oct 2022 15:36
 Operator : SY/MD
 Sample : N5233-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA56

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	95	rBV	107988	117698	17.71%	2.120%
2	1.568	156	164	180	rVB	101549	120122	18.08%	2.164%
3	2.105	320	331	345	rVB	192086	281739	42.40%	5.075%
4	2.503	447	455	466	rBV5	6939	12405	1.87%	0.223%
5	2.767	524	537	551	rVB3	19610	40431	6.08%	0.728%
6	3.918	884	895	924	rBV2	45749	215457	32.42%	3.881%
7	4.352	1011	1030	1061	rBV5	137739	464419	69.89%	8.366%
8	5.043	1230	1245	1275	rBV2	266959	664506	100.00%	11.971%
9	5.616	1411	1423	1445	rBV	217937	455697	68.58%	8.209%
10	6.066	1548	1563	1590	rBV	154373	332236	50.00%	5.985%
11	6.989	1838	1850	1861	rBV	34745	69045	10.39%	1.244%
12	7.313	1940	1951	1974	rBV	287799	515265	77.54%	9.282%
13	7.629	2041	2049	2059	rBV3	18637	35187	5.30%	0.634%
14	8.095	2183	2194	2224	rBV3	251190	610356	91.85%	10.995%
15	8.847	2415	2428	2451	rBV	332327	565828	85.15%	10.193%
16	10.210	2836	2852	2866	rBV	96723	161171	24.25%	2.903%
17	10.378	2894	2904	2910	rBV5	8614	13609	2.05%	0.245%
18	11.243	3162	3173	3195	rBV	300635	481819	72.51%	8.680%
19	11.532	3257	3263	3270	rBV	4369	7964	1.20%	0.143%
20	11.619	3278	3290	3312	rBV	233424	386104	58.10%	6.956%




Sum of corrected areas: 5551058

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028721.D
Acq On : 27 Oct 2022 15:36
Operator : SY/MD
Sample : N5233-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

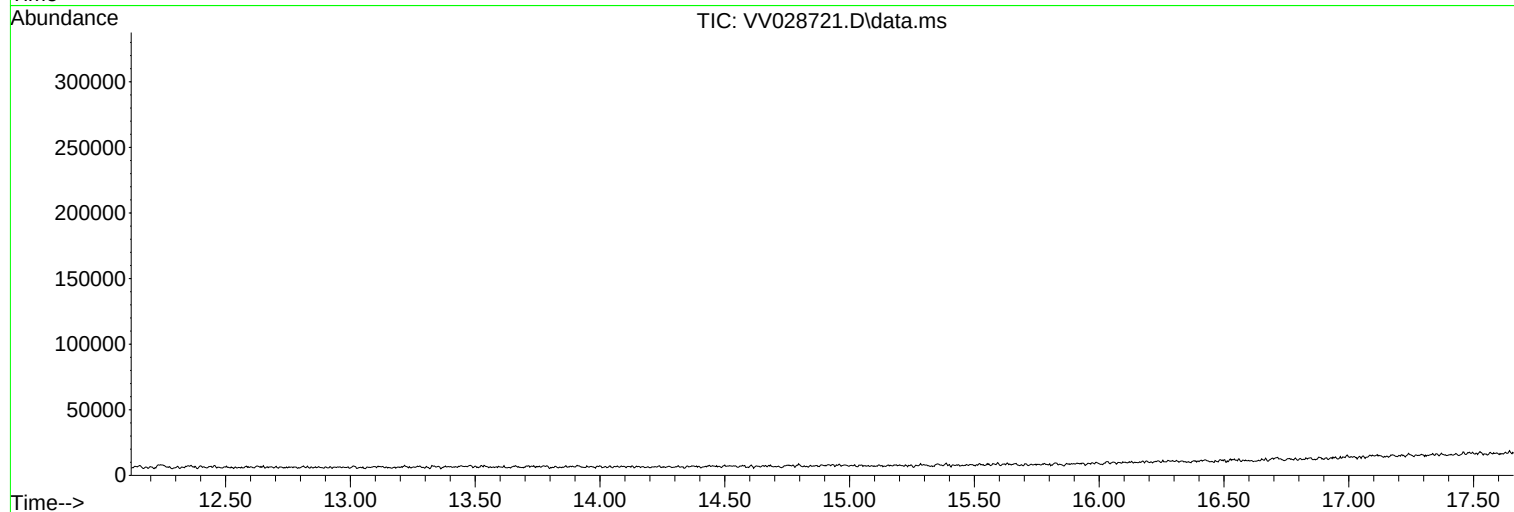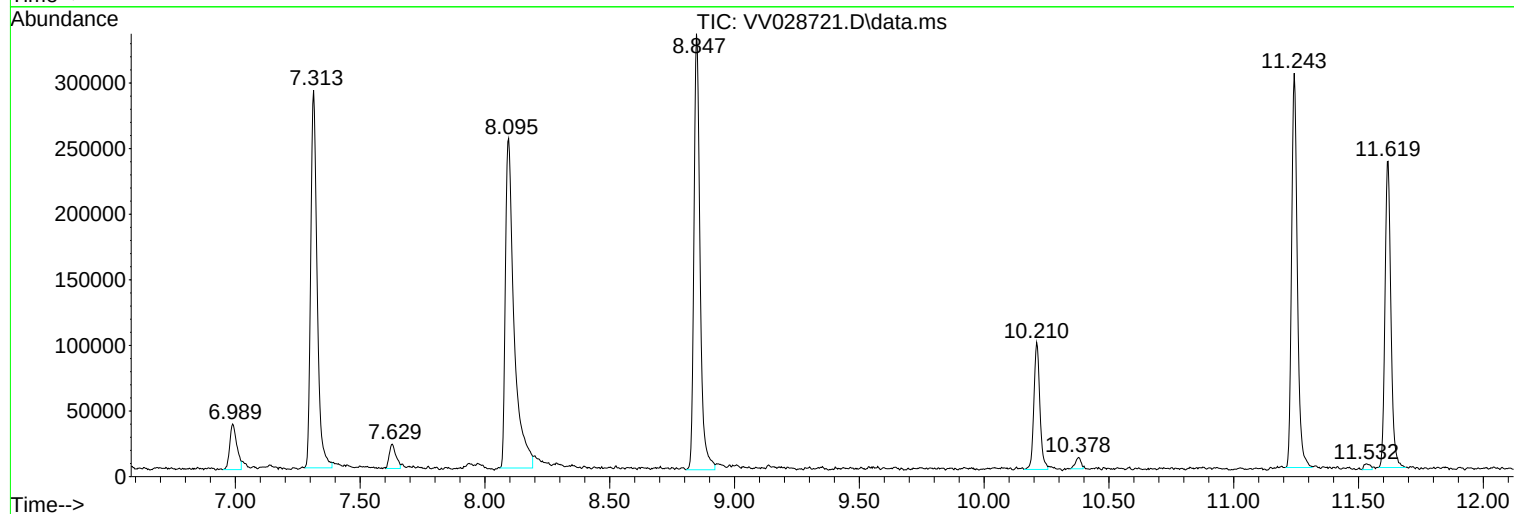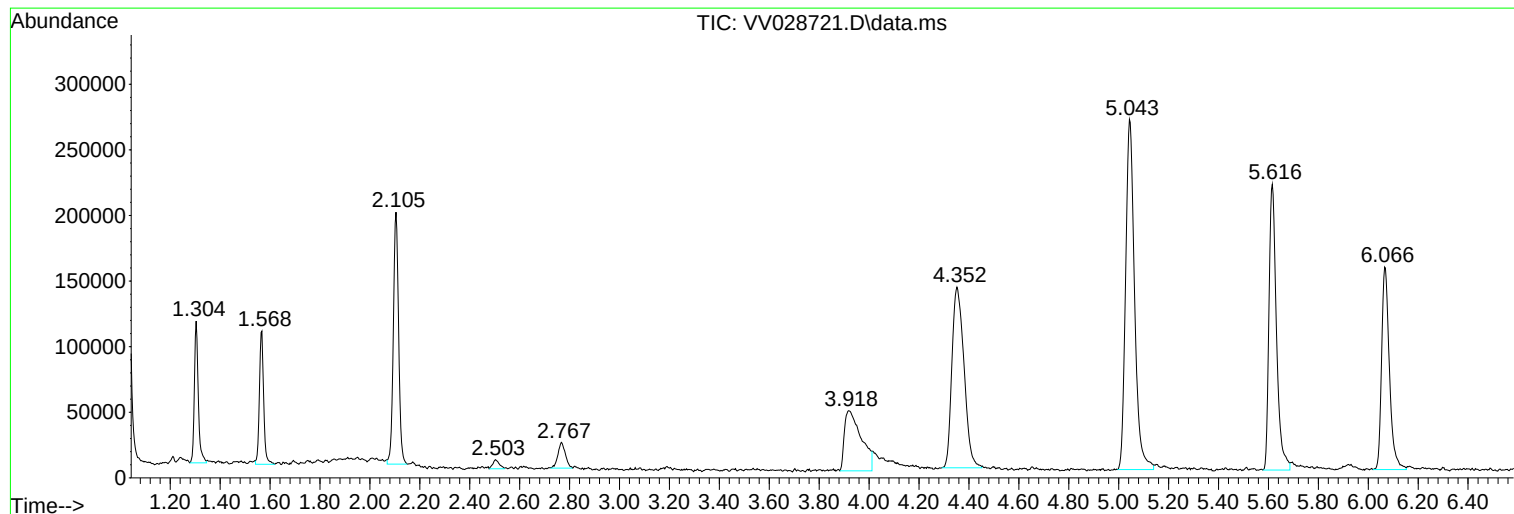

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028721.D
Acq On : 27 Oct 2022 15:36
Operator : SY/MD
Sample : N5233-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028721.D
Acq On : 27 Oct 2022 15:36
Operator : SY/MD
Sample : N5233-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc