

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
 Data File : VV028725.D
 Acq On : 27 Oct 2022 17:40
 Operator : SY/MD
 Sample : VIBLK303
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK303

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	108232	109271	12.16%	1.447%
2	1.564	157	163	172	rBV	115076	132643	14.76%	1.756%
3	2.105	322	331	348	rVB	229130	349794	38.91%	4.631%
4	2.503	439	455	465	rBV	34902	62301	6.93%	0.825%
5	3.034	614	620	635	rVB	6239	13223	1.47%	0.175%
6	3.899	874	889	925	rBV3	99410	402075	44.73%	5.323%
7	4.342	1009	1027	1048	rBV	137034	348609	38.78%	4.615%
8	5.043	1228	1245	1278	rBV2	322971	898962	100.00%	11.900%
9	5.612	1410	1422	1442	rBV	318494	655646	72.93%	8.679%
10	6.066	1549	1563	1582	rBV2	187764	403656	44.90%	5.344%
11	6.985	1840	1849	1869	rBV2	60204	117962	13.12%	1.562%
12	7.310	1939	1950	1966	rBV	348056	628489	69.91%	8.320%
13	7.387	1967	1974	1991	rVB2	34754	72962	8.12%	0.966%
14	7.622	2039	2047	2062	rBV3	30938	58784	6.54%	0.778%
15	8.088	2181	2192	2223	rBV	338003	765817	85.19%	10.138%
16	8.847	2416	2428	2457	rBV	466100	800236	89.02%	10.594%
17	9.014	2470	2480	2489	rBV	23795	40096	4.46%	0.531%
18	9.133	2507	2517	2533	rBV	83834	135670	15.09%	1.796%
19	9.545	2637	2645	2650	rBV3	8135	12211	1.36%	0.162%
20	10.210	2835	2852	2871	rVB	117330	200997	22.36%	2.661%
21	10.911	3062	3070	3080	rBV2	13196	24648	2.74%	0.326%
22	11.242	3162	3173	3192	rBV	441388	708548	78.82%	9.380%
23	11.332	3195	3201	3215	rVB	7057	14014	1.56%	0.186%
24	11.619	3276	3290	3307	rBV	304450	506851	56.38%	6.710%
25	11.966	3391	3398	3406	rBV	6597	10340	1.15%	0.137%
26	13.152	3760	3767	3780	rVB	8692	14167	1.58%	0.188%
27	13.258	3791	3800	3813	rVB	7106	11633	1.29%	0.154%
28	13.500	3865	3875	3888	rBV2	14888	28579	3.18%	0.378%
29	13.738	3939	3949	3963	rBV2	7258	13418	1.49%	0.178%
30	16.168	4696	4705	4712	rBV2	6800	12418	1.38%	0.164%




Sum of corrected areas: 7554020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028725.D
Acq On : 27 Oct 2022 17:40
Operator : SY/MD
Sample : VIBLK303
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

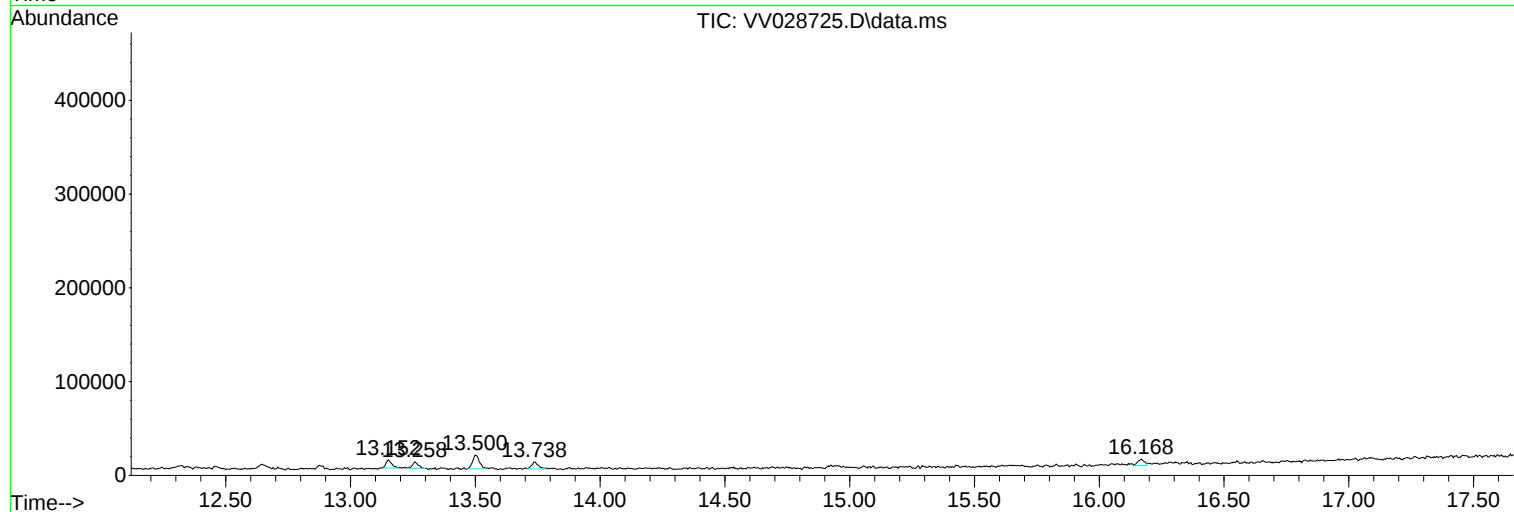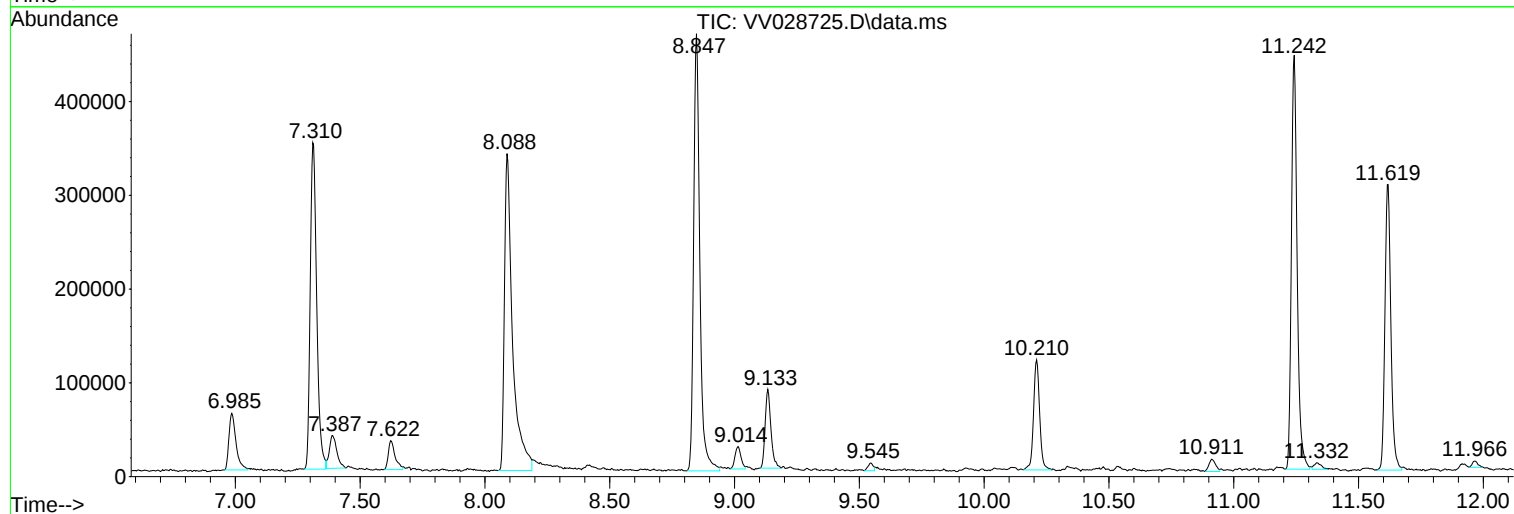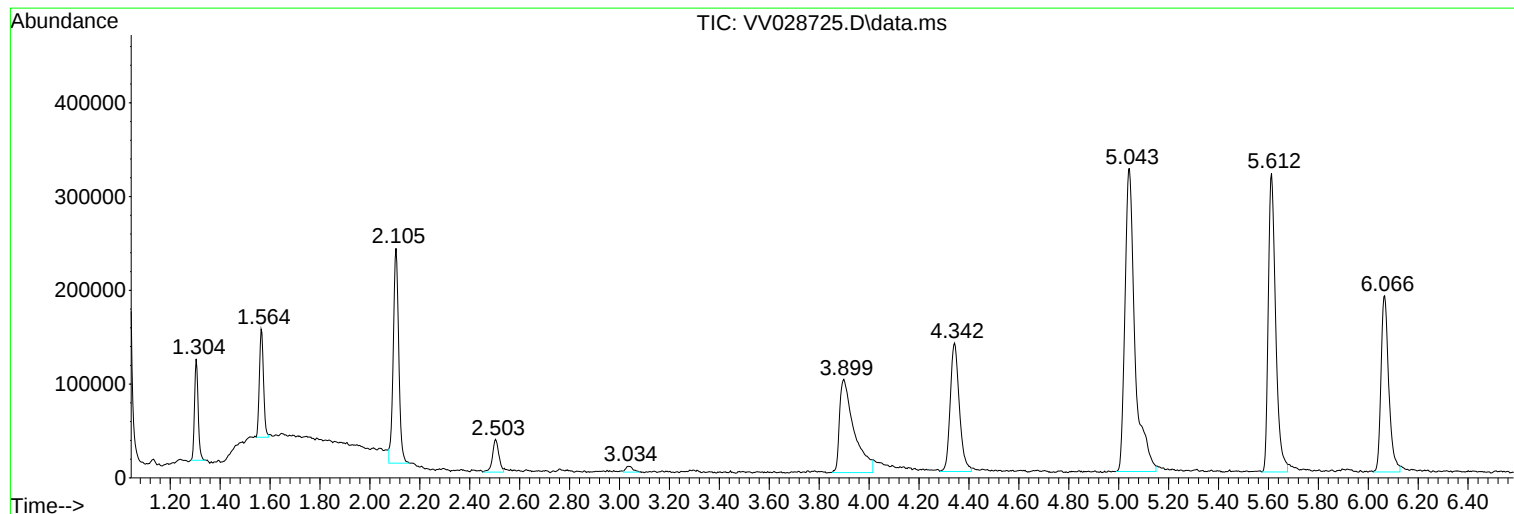

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028725.D
Acq On : 27 Oct 2022 17:40
Operator : SY/MD
Sample : VIBLK303
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028725.D
Acq On : 27 Oct 2022 17:40
Operator : SY/MD
Sample : VIBLK303
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc