

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
 Data File : VV028729.D
 Acq On : 27 Oct 2022 19:18
 Operator : SY/MD
 Sample : N5233-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA62

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	100	rBV	120689	133254	15.94%	2.032%
2	1.474	120	135	137	rBV	21558	44183	5.29%	0.674%
3	1.568	157	164	177	rVB	119639	138018	16.51%	2.105%
4	2.105	322	331	352	rVB	228902	355882	42.58%	5.428%
5	2.503	450	455	465	rVB7	6363	9056	1.08%	0.138%
6	3.905	876	891	931	rBV2	73273	314502	37.63%	4.797%
7	4.346	1007	1028	1050	rBV	136739	365439	43.73%	5.573%
8	5.043	1229	1245	1280	rBV2	325184	835737	100.00%	12.746%
9	5.616	1411	1423	1445	rBV	257614	533507	63.84%	8.137%
10	6.066	1550	1563	1582	rBV	190697	395801	47.36%	6.037%
11	6.989	1838	1850	1864	rBV2	40750	80548	9.64%	1.228%
12	7.313	1936	1951	1970	rBV	348660	624805	74.76%	9.529%
13	7.394	1973	1976	1987	rVB6	7616	11561	1.38%	0.176%
14	7.625	2037	2048	2062	rBV3	20334	41342	4.95%	0.631%
15	8.091	2181	2193	2240	rBV3	320137	753219	90.13%	11.488%
16	8.847	2417	2428	2453	rBV	391676	662198	79.24%	10.099%
17	9.136	2507	2518	2531	rBV	17379	31470	3.77%	0.480%
18	10.210	2839	2852	2870	rBV	116130	186814	22.35%	2.849%
19	11.242	3161	3173	3195	rBV	346216	568651	68.04%	8.673%
20	11.619	3276	3290	3308	rBV	282455	470803	56.33%	7.180%




Sum of corrected areas: 6556790

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028729.D
Acq On : 27 Oct 2022 19:18
Operator : SY/MD
Sample : N5233-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

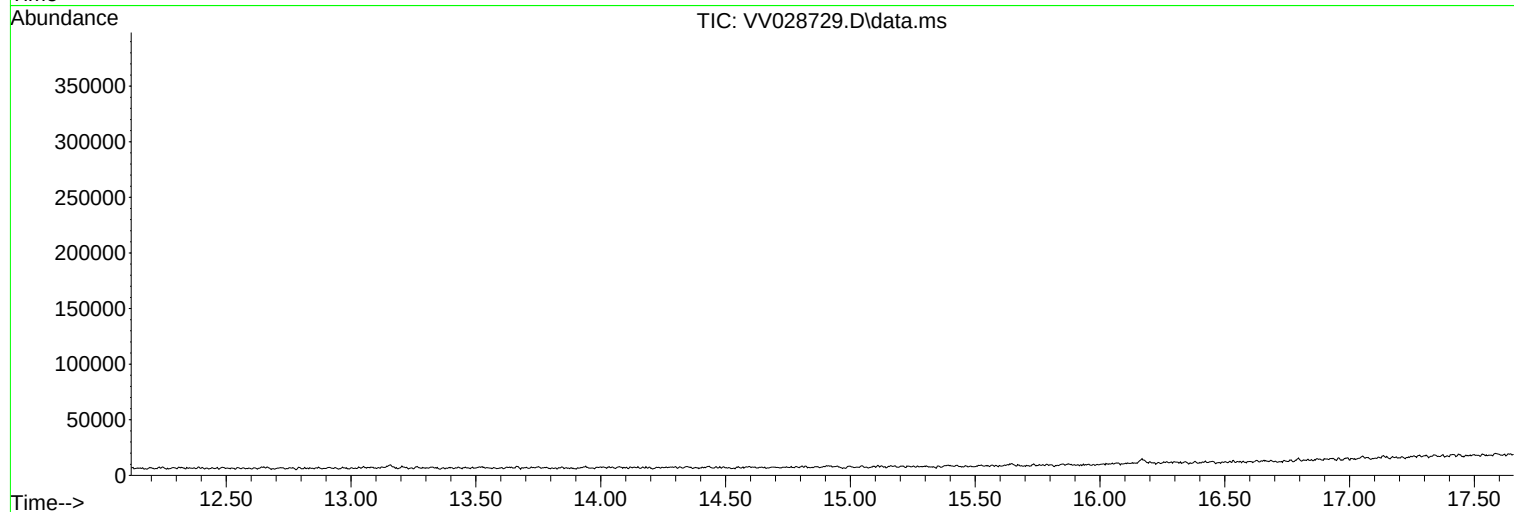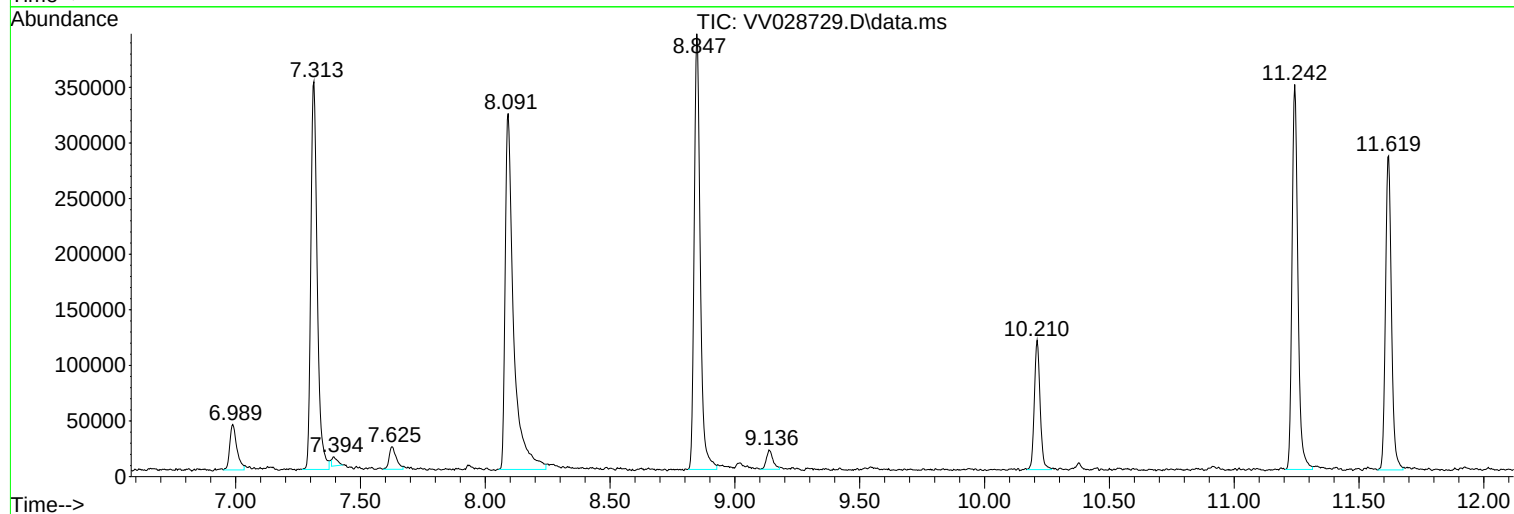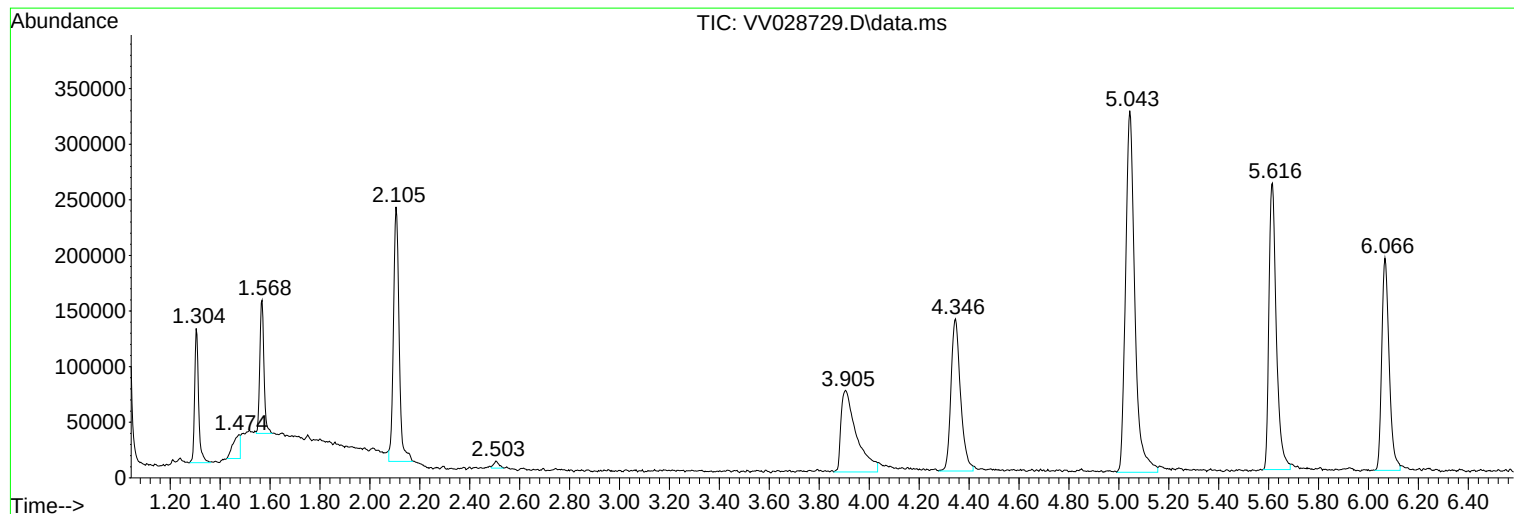

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028729.D
Acq On : 27 Oct 2022 19:18
Operator : SY/MD
Sample : N5233-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028729.D
Acq On : 27 Oct 2022 19:18
Operator : SY/MD
Sample : N5233-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
