

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
 Data File : VV028738.D
 Acq On : 28 Oct 2022 00:16
 Operator : SY/MD
 Sample : N5232-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAD3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	74627	81196	10.71%	1.311%
2	1.494	123	141	145	rBV2	25014	69847	9.21%	1.128%
3	1.568	157	164	173	rVB	82257	95022	12.53%	1.534%
4	2.105	322	331	343	rVB	144007	214267	28.26%	3.460%
5	2.179	347	354	369	rVB3	9839	22353	2.95%	0.361%
6	3.889	875	886	924	rBV	92695	329028	43.40%	5.313%
7	4.352	1010	1030	1059	rBV4	133770	465239	61.37%	7.512%
8	5.043	1231	1245	1265	rBV2	231057	589872	77.81%	9.525%
9	5.612	1409	1422	1447	rBV	265768	556011	73.34%	8.978%
10	6.066	1549	1563	1588	rBV	150843	315512	41.62%	5.095%
11	6.985	1838	1849	1865	rBV2	54277	108584	14.32%	1.753%
12	7.313	1939	1951	1968	rBV	248875	443821	58.55%	7.166%
13	7.391	1968	1975	1988	rVB2	15359	31733	4.19%	0.512%
14	7.622	2040	2047	2062	rBV2	26383	48823	6.44%	0.788%
15	8.088	2181	2192	2229	rBV	355208	758078	100.00%	12.241%
16	8.255	2235	2244	2254	rVB	8175	15230	2.01%	0.246%
17	8.847	2416	2428	2451	rBV	400347	728405	96.09%	11.762%
18	9.140	2507	2519	2527	rBV3	11857	23556	3.11%	0.380%
19	9.545	2636	2645	2650	rBV3	5847	9221	1.22%	0.149%
20	9.924	2754	2763	2777	rBV3	9868	18179	2.40%	0.294%
21	10.210	2839	2852	2864	rBV	106723	172035	22.69%	2.778%
22	10.371	2896	2902	2912	rVB5	8179	14181	1.87%	0.229%
23	11.242	3161	3173	3197	rBV	385904	609214	80.36%	9.837%
24	11.529	3251	3262	3270	rBV	8217	16248	2.14%	0.262%
25	11.615	3275	3289	3306	rBV	232495	392363	51.76%	6.336%
26	12.345	3509	3516	3527	rVB	7872	14098	1.86%	0.228%
27	16.297	4734	4745	4757	rBV3	29228	50956	6.72%	0.823%




Sum of corrected areas: 6193072

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028738.D
Acq On : 28 Oct 2022 00:16
Operator : SY/MD
Sample : N5232-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

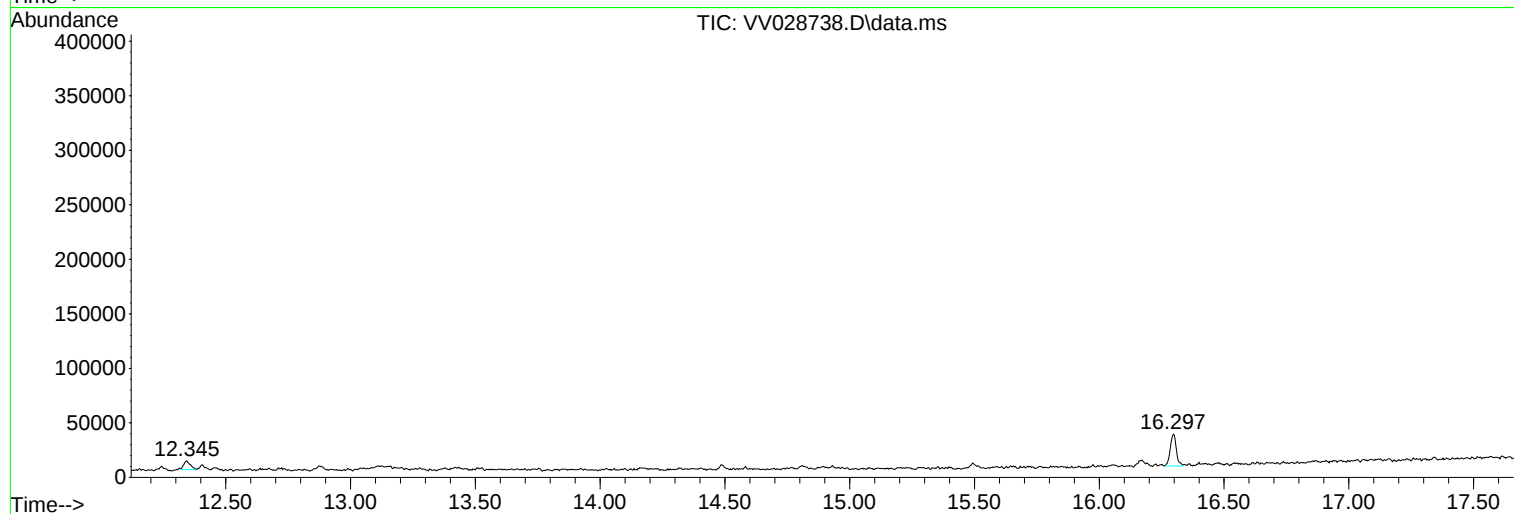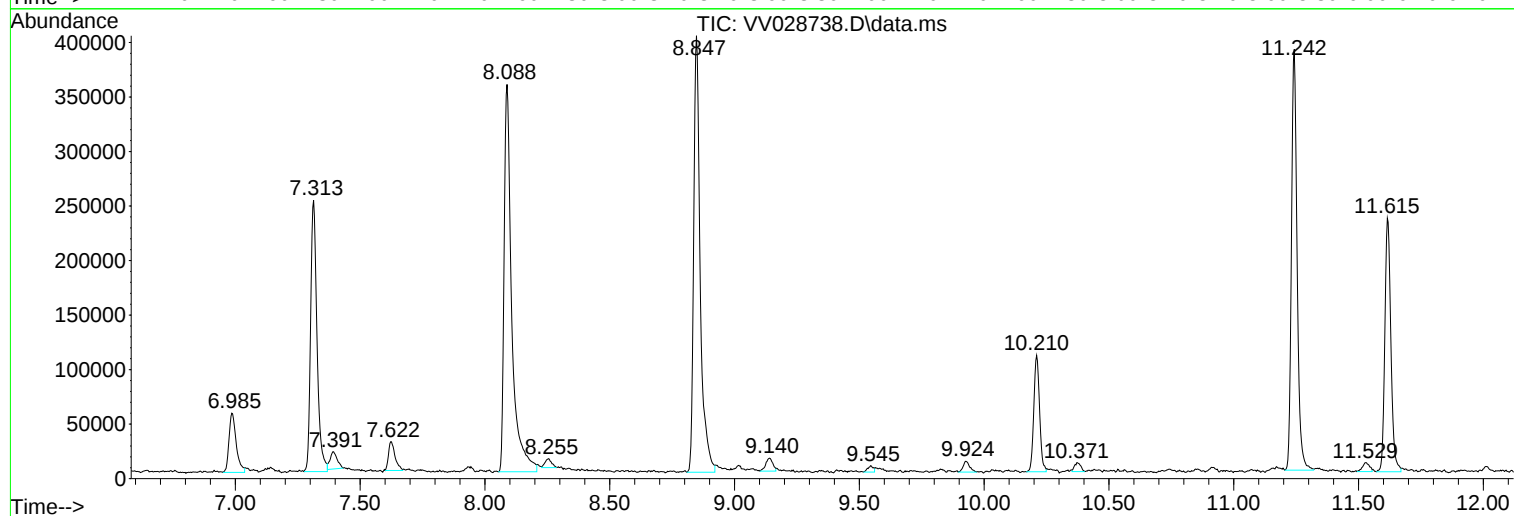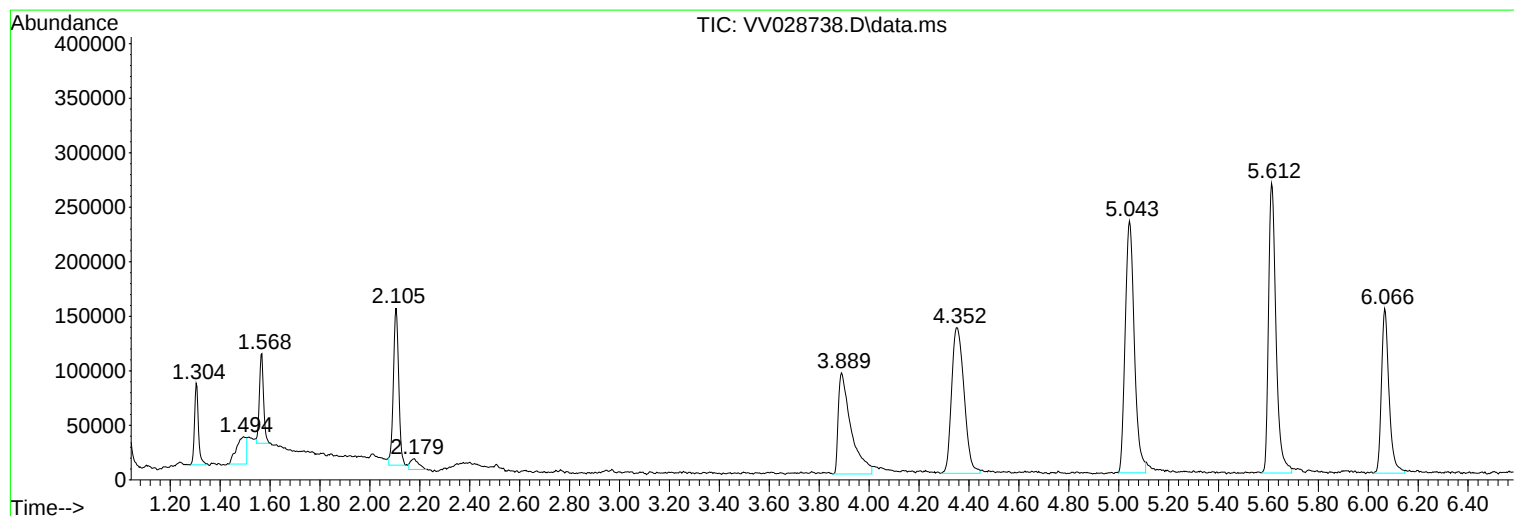

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028738.D
Acq On : 28 Oct 2022 00:16
Operator : SY/MD
Sample : N5232-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.494	0.6	ug/L	69847	1	5.612	556011	5.0