

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
 Data File : VV028739.D
 Acq On : 28 Oct 2022 00:41
 Operator : SY/MD
 Sample : N5232-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAD4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	98	rBV	107008	117454	10.18%	1.534%
2	1.565	156	163	173	rBV	114757	133314	11.56%	1.741%
3	2.101	321	330	346	rVB	211171	312767	27.11%	4.084%
4	3.899	878	889	918	rBV2	92802	360998	31.29%	4.714%
5	4.349	1011	1029	1056	rBV3	177586	569291	49.35%	7.434%
6	5.043	1229	1245	1275	rBV2	347548	892734	77.38%	11.657%
7	5.613	1408	1422	1447	rBV	258688	546459	47.37%	7.136%
8	6.066	1551	1563	1583	rBV	217252	453513	39.31%	5.922%
9	6.986	1839	1849	1866	rBV	82170	159652	13.84%	2.085%
10	7.310	1937	1950	1968	rBV	369042	660419	57.24%	8.624%
11	7.394	1968	1976	1993	rVB	18120	40272	3.49%	0.526%
12	7.622	2036	2047	2066	rBV	43339	89182	7.73%	1.165%
13	8.088	2180	2192	2231	rBV	523635	1153676	100.00%	15.065%
14	8.847	2415	2428	2450	rBV	386315	677352	58.71%	8.845%
15	9.140	2509	2519	2530	rBV5	11443	22150	1.92%	0.289%
16	9.551	2637	2647	2658	rBV5	5835	13628	1.18%	0.178%
17	10.210	2842	2852	2869	rBV	159016	251592	21.81%	3.285%
18	11.243	3162	3173	3195	rBV	372062	594053	51.49%	7.757%
19	11.616	3278	3289	3304	rBV	354451	564376	48.92%	7.370%
20	12.342	3508	3515	3528	rBV	9146	17242	1.49%	0.225%
21	16.297	4736	4745	4752	rBV4	18794	28020	2.43%	0.366%




Sum of corrected areas: 7658144

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028739.D
Acq On : 28 Oct 2022 00:41
Operator : SY/MD
Sample : N5232-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

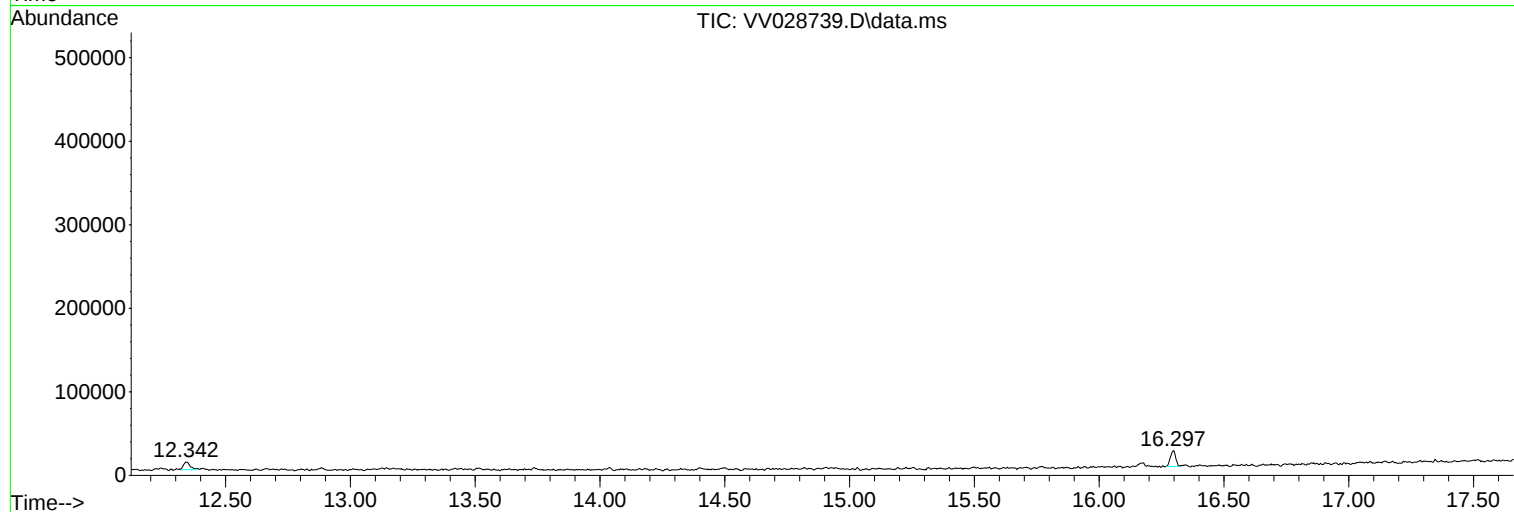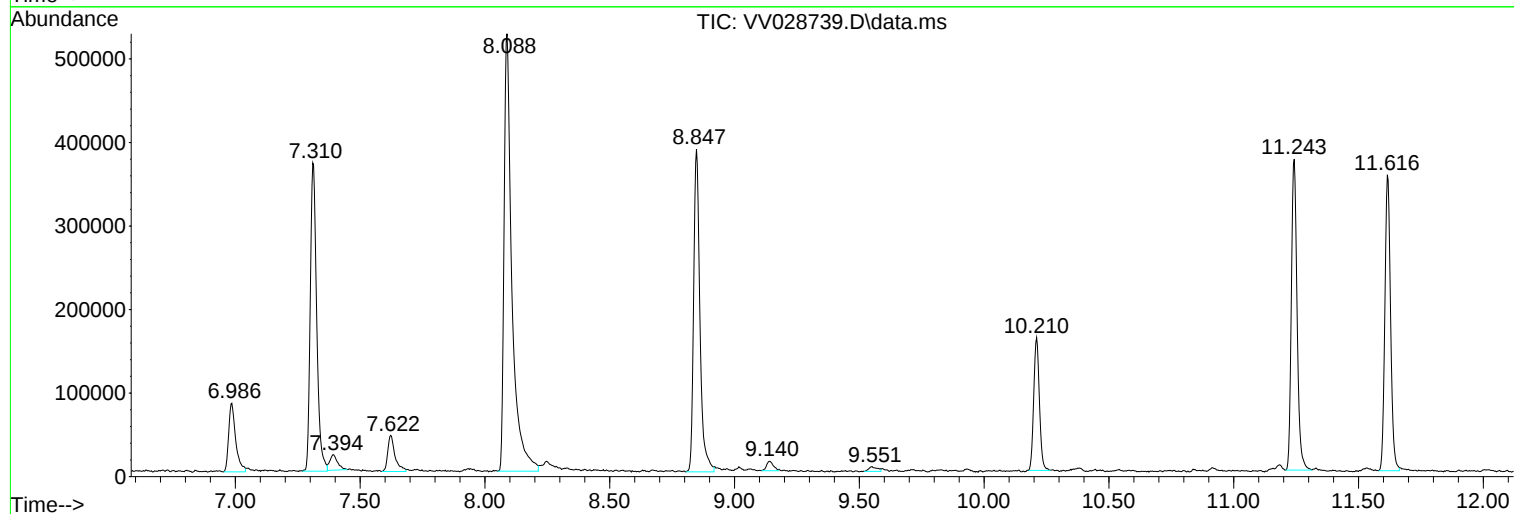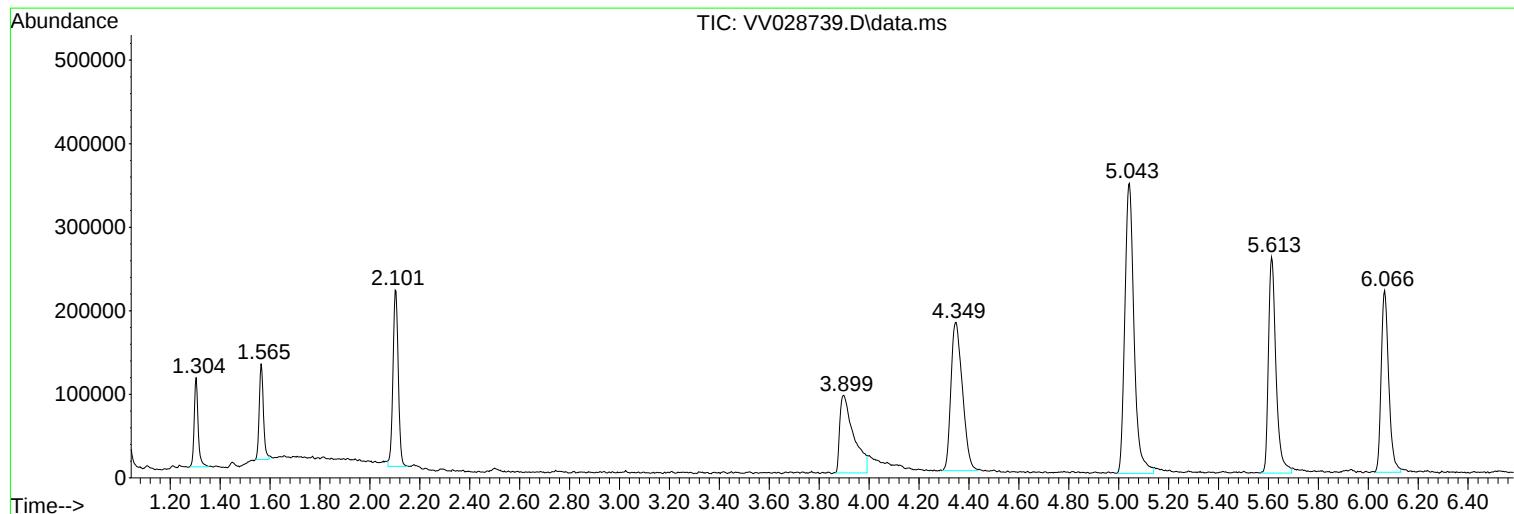

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028739.D
Acq On : 28 Oct 2022 00:41
Operator : SY/MD
Sample : N5232-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
Data File : VV028739.D
Acq On : 28 Oct 2022 00:41
Operator : SY/MD
Sample : N5232-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc