


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102722\
 Data File : VV028708.D
 Acq On : 27 Oct 2022 09:16
 Operator : SY/MD
 Sample : BFB392
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB392

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Oct 28 21:50:06 2022

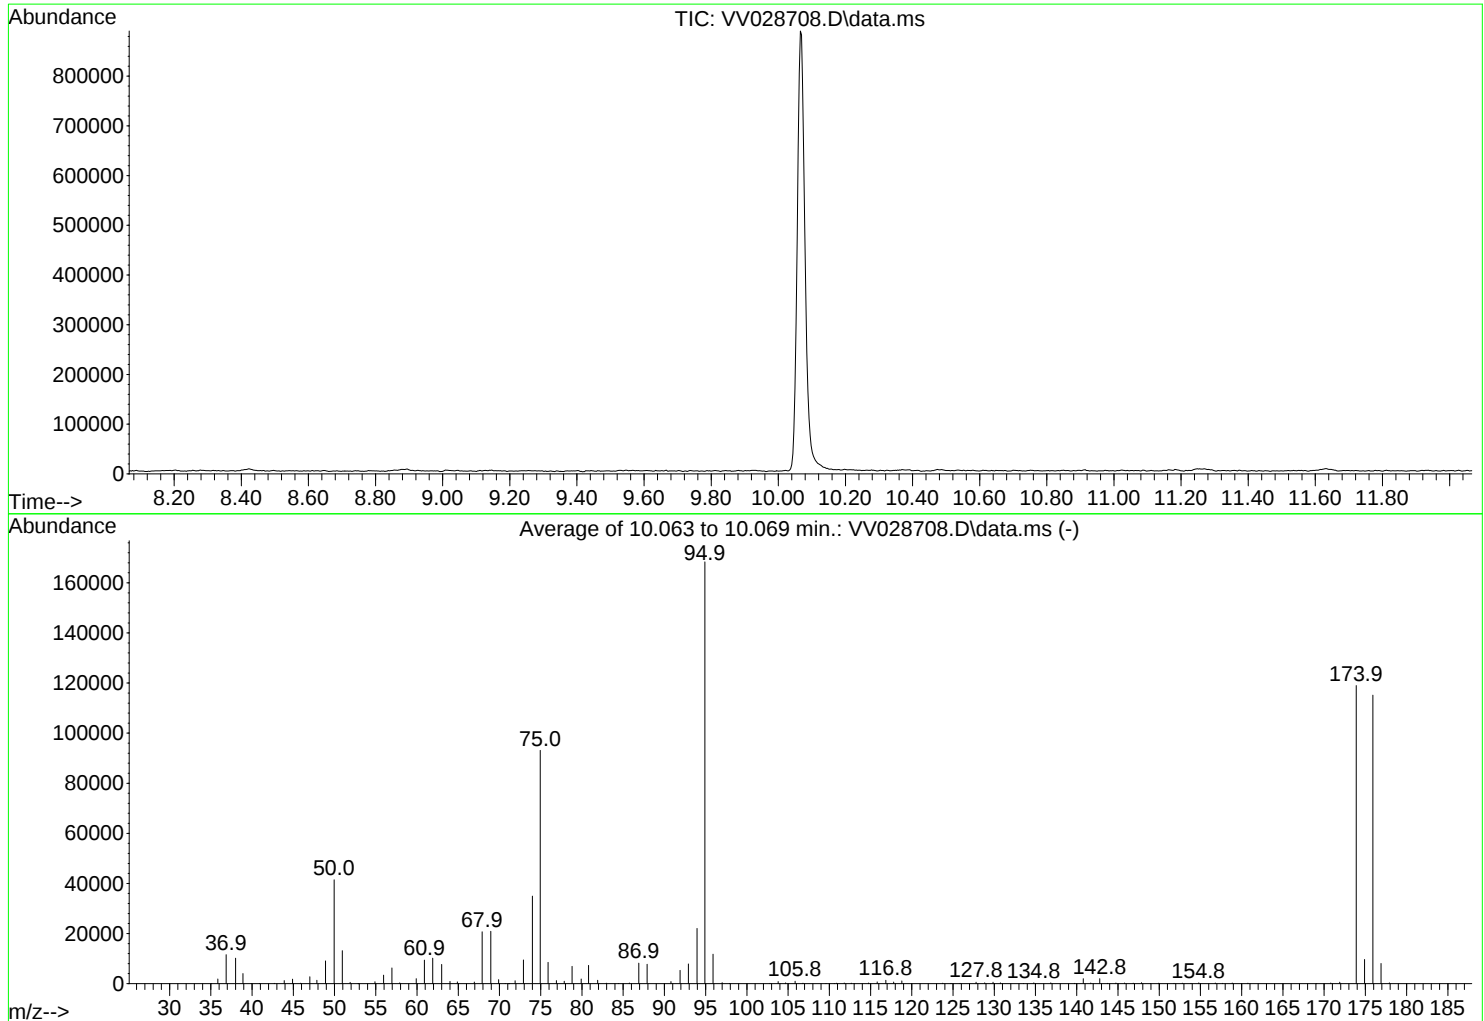

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	41432	PASS
75	95	30	80	55.3	93104	PASS
95	95	100	100	100.0	168384	PASS
96	95	5	9	7.0	11751	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.7	118995	PASS
175	174	5	9	8.1	9616	PASS
176	174	95	105	96.8	115187	PASS
177	176	5	10	7.0	8047	PASS

m/z	Abundance
35.40	164.0
35.90	210.0
36.80	158.0
37.70	157.0
38.00	154.0
38.90	199.0
39.90	1123.0
40.90	127.0
41.90	182.0
42.60	143.0
43.90	689.0
44.90	183.0
45.90	140.0
47.70	147.0
48.30	162.0
49.00	125.0
50.50	133.0
51.40	136.0
52.90	121.0
53.50	181.0
54.10	101.0
54.60	122.0
55.30	127.0
56.00	109.0
56.90	145.0
57.50	122.0
58.40	124.0
60.10	151.0
60.60	114.0
63.10	110.0
65.80	133.0
78.30	117.0
80.40	128.0
83.70	112.0
87.90	113.0
99.90	114.0
123.10	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

m/z	Abundance
35.10	132.0
35.90	1993.0
36.90	11368.0
38.00	9820.0
39.00	4019.0
39.90	1199.0
41.00	185.0
41.90	180.0
42.80	268.0
43.90	1829.0
44.90	2044.0
45.90	308.0
47.00	2756.0
47.90	1444.0
48.90	8692.0
49.90	39920.0
51.00	12955.0
51.90	525.0
52.90	135.0
53.70	135.0
54.90	668.0
55.90	3397.0
57.00	6019.0
57.90	324.0
59.90	2061.0
60.90	9223.0
61.90	9336.0
63.00	7314.0
64.00	797.0
64.90	799.0
66.90	594.0
67.90	20008.0
68.90	20160.0
69.90	1464.0
71.90	1095.0
72.90	8946.0
74.00	33336.0
74.90	88224.0
75.90	8052.0
76.90	1081.0
77.90	978.0
78.80	6742.0
79.90	1664.0
80.80	6869.0
81.90	1228.0
83.00	204.0
84.40	119.0
85.80	261.0
86.90	7560.0
87.90	7369.0
90.80	757.0
91.90	4856.0
92.90	7531.0
93.90	20584.0
94.90	158592.0
95.90	11087.0
97.00	389.0
102.80	144.0
103.70	775.0
104.70	307.0
105.80	893.0
106.80	146.0
110.80	175.0
111.80	230.0
112.70	214.0
114.80	243.0
115.80	722.0
116.90	1271.0
117.80	586.0
118.80	1138.0
123.80	180.0
124.80	104.0
125.90	117.0
127.80	568.0
128.80	294.0
129.80	534.0
130.80	257.0
134.90	273.0
136.80	336.0
139.80	171.0
140.80	1775.0
141.70	291.0
142.80	1860.0
143.80	113.0
144.70	228.0
145.80	245.0
146.90	177.0
147.90	395.0
148.90	103.0
149.90	256.0
151.80	123.0
152.80	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

153.80	139.0
154.80	373.0
156.80	249.0
157.70	115.0
158.90	262.0
160.70	214.0
170.80	217.0
172.00	631.0
173.90	107968.0
174.90	9205.0
175.90	104472.0
176.90	7374.0
177.90	307.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

m/z	Abundance
35.90	2100.0
36.90	12158.0
38.00	10695.0
38.90	4387.0
39.90	1139.0
40.90	189.0
42.00	184.0
42.80	306.0
43.90	1861.0
44.90	2062.0
45.90	357.0
47.00	2773.0
47.90	1571.0
48.90	9432.0
50.00	42864.0
50.90	13671.0
51.90	530.0
52.90	134.0
53.70	144.0
54.90	787.0
56.00	3619.0
57.00	6682.0
57.90	377.0
59.90	2160.0
60.90	9730.0
61.90	10551.0
63.00	8059.0
64.00	910.0
64.90	743.0
67.00	636.0
67.90	21560.0
69.00	21600.0
69.90	1622.0
71.10	106.0
71.90	1229.0
72.90	9912.0
74.00	36280.0
75.00	96248.0
75.90	8796.0
76.90	1257.0
77.90	1078.0
78.80	7170.0
79.90	1943.0
80.80	7623.0
81.90	1391.0
83.00	236.0
84.50	122.0
85.80	246.0
86.90	8392.0
87.90	8198.0
90.80	870.0
91.90	5504.0
92.90	8173.0
93.90	22920.0
94.90	174208.0
95.90	12319.0
97.00	397.0
97.90	106.0
102.80	158.0
103.80	844.0
104.70	350.0
105.90	1006.0
106.80	177.0
110.90	176.0
111.80	242.0
112.60	207.0
114.70	255.0
115.80	741.0
116.80	1436.0
117.80	658.0
118.80	1138.0
123.80	191.0
124.80	110.0
125.80	126.0
127.80	645.0
128.90	336.0
129.80	555.0
130.80	315.0
133.60	118.0
134.80	303.0
136.80	356.0
139.80	159.0
140.80	2057.0
141.70	261.0
142.80	2056.0
143.70	140.0
144.80	261.0
145.80	255.0
146.90	198.0
147.90	419.0
149.90	239.0
151.80	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

152.80	188.0
153.90	145.0
154.80	367.0
156.80	301.0
157.70	142.0
158.90	262.0
160.80	196.0
170.80	277.0
171.80	599.0
173.90	123216.0
174.90	9987.0
175.90	119376.0
176.90	8472.0
177.90	321.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

m/z	Abundance
35.90	2139.0
36.90	11564.0
38.00	10357.0
38.90	4251.0
39.90	1173.0
40.90	191.0
42.00	171.0
42.80	294.0
43.90	1981.0
44.90	1900.0
45.90	342.0
47.00	2641.0
47.90	1435.0
48.90	9437.0
50.00	41512.0
50.90	12874.0
51.90	521.0
52.70	141.0
53.70	153.0
54.90	865.0
56.00	3458.0
57.00	6435.0
57.90	367.0
59.90	2100.0
60.90	9292.0
61.90	10548.0
63.00	7968.0
64.00	1027.0
64.90	593.0
65.80	105.0
67.00	619.0
67.90	20560.0
68.90	20872.0
69.90	1701.0
70.70	192.0
71.90	1196.0
72.90	9582.0
74.00	35200.0
75.00	94840.0
75.90	8666.0
76.90	1353.0
77.80	942.0
78.80	6786.0
79.90	1982.0
80.80	7463.0
81.90	1442.0
82.90	252.0
83.80	129.0
85.70	215.0
86.90	8596.0
87.90	8071.0
90.80	889.0
91.90	5626.0
92.90	7815.0
94.00	22600.0
94.90	172352.0
95.90	11846.0
97.00	341.0
97.90	141.0
102.80	164.0
103.90	872.0
104.70	368.0
105.80	1012.0
106.80	181.0
109.60	145.0
110.60	167.0
111.00	200.0
111.80	243.0
112.60	203.0
113.00	178.0
114.80	255.0
115.80	707.0
116.80	1368.0
117.80	708.0
118.80	961.0
123.70	177.0
124.70	109.0
125.80	141.0
127.80	607.0
128.90	319.0
129.90	566.0
130.70	319.0
133.50	107.0
134.70	315.0
136.90	360.0
139.70	122.0
140.80	2056.0
141.70	220.0
142.80	1990.0
143.80	137.0
144.80	295.0
145.80	264.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

146.80	179.0
147.80	365.0
149.00	120.0
150.00	199.0
151.80	102.0
152.80	172.0
153.90	184.0
154.80	328.0
156.80	323.0
157.70	119.0
158.70	245.0
160.80	193.0
169.10	138.0
170.80	291.0
171.90	586.0
173.90	125800.0
174.90	9655.0
175.90	121712.0
176.90	8295.0
177.90	292.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392