

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110724\
 Data File : VV037959.D
 Acq On : 07 Nov 2024 16:45
 Operator : SY/MD
 Sample : P4715-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAM6

Quant Time: Nov 08 01:29:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 08 01:25:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	255951	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	278702	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	118890	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	94376	4.817	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.400%
7) Chloroethane-d5	1.529	69	74885	4.690	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.800%
11) 1,1-Dichloroethene-d2	2.053	65	40664	4.783	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.600%
20) 2-Butanone-d5	3.805	46	159406	43.656	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.320%
24) Chloroform-d	4.243	84	179652	5.031	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	4.940	65	85018	5.327	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.600%
32) Benzene-d6	4.953	84	331922	4.618	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.400%
36) 1,2-Dichloropropane-d6	5.985	67	104555	4.981	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.600%
41) Toluene-d8	7.239	98	279981	4.334	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
43) trans-1,3-Dichloroprop...	7.561	79	32165	3.963	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.200%
46) 2-Hexanone-d5	8.027	63	149265	47.327	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.660%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	89075	5.264	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.200%
66) 1,2-Dichlorobenzene-d4	11.554	152	109845	5.602	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.000%
Target Compounds						Qvalue
13) Acetone	2.133	43	27130	10.467	ug/L	99
16) Methylene chloride	2.442	84	441732	21.643	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110724\
Data File : VV037959.D
Acq On : 07 Nov 2024 16:45
Operator : SY/MD
Sample : P4715-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAM6

Quant Time: Nov 08 01:29:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 08 01:25:43 2024
Response via : Initial Calibration

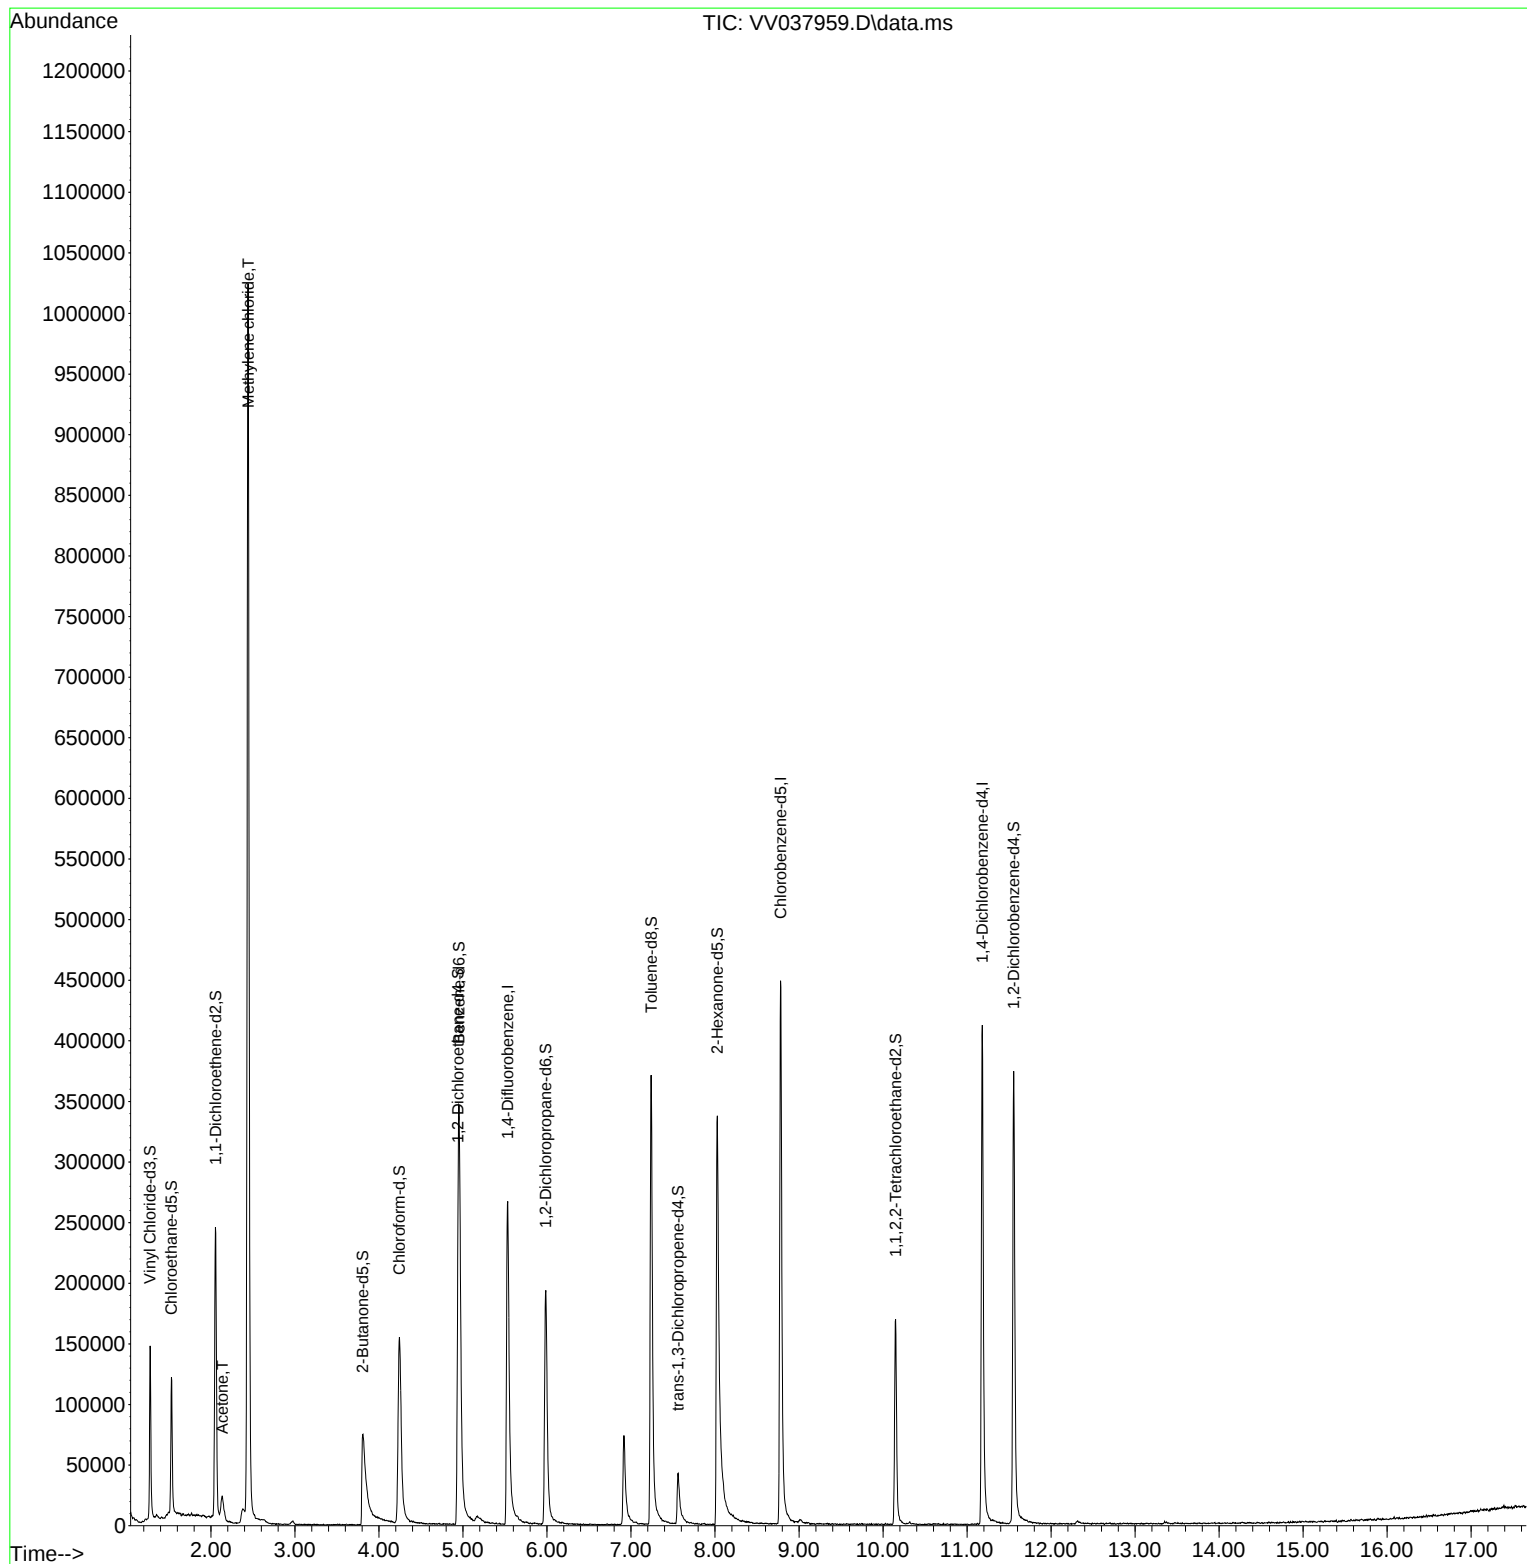

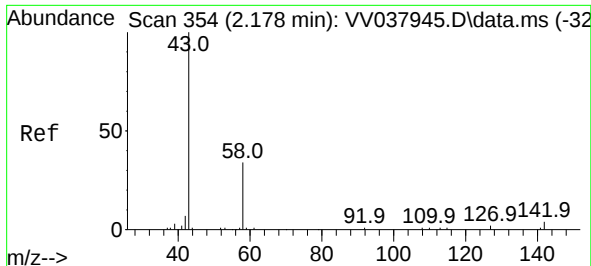

#13

Acetone

Concen: 10.467 ug/L

RT: 2.133 min Scan# 34

Delta R.T. -0.045 min

Lab File: VV037959.D

Acq: 07 Nov 2024 16:45

Instrument :

MSVOA_V

ClientSampleId :





COAM6

Tgt Ion: 43 Resp: 27130

Ion Ratio Lower Upper

43 100

58 33.1 0.0 64.6

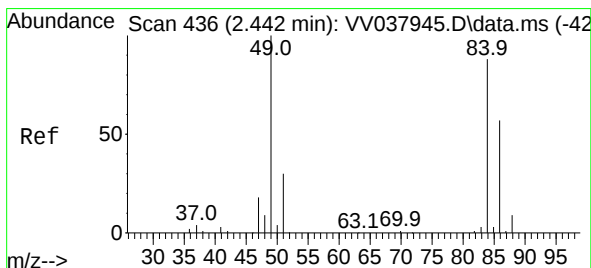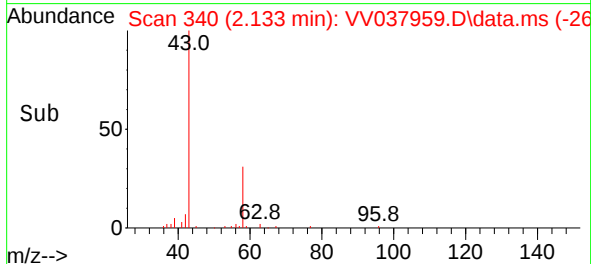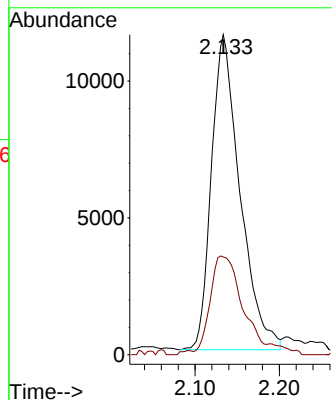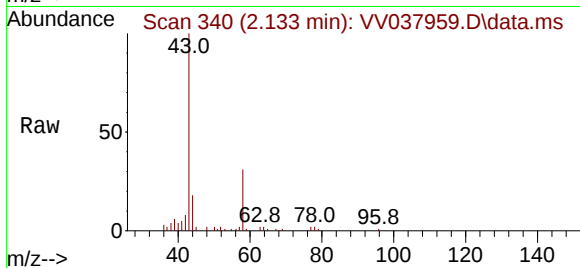

#16

Methylene chloride

Concen: 21.643 ug/L

RT: 2.442 min Scan# 436

Delta R.T. -0.000 min

Lab File: VV037959.D

Acq: 07 Nov 2024 16:45

Tgt Ion: 84 Resp: 441732

Ion Ratio Lower Upper

84 100

86 65.1 45.0 83.6

49 112.8 79.2 147.2

