


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110724\
Data File : VV037944.D
Acq On : 07 Nov 2024 08:53
Operator : SY/MD
Sample : BFB282
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB282

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Nov 09 02:20:30 2024

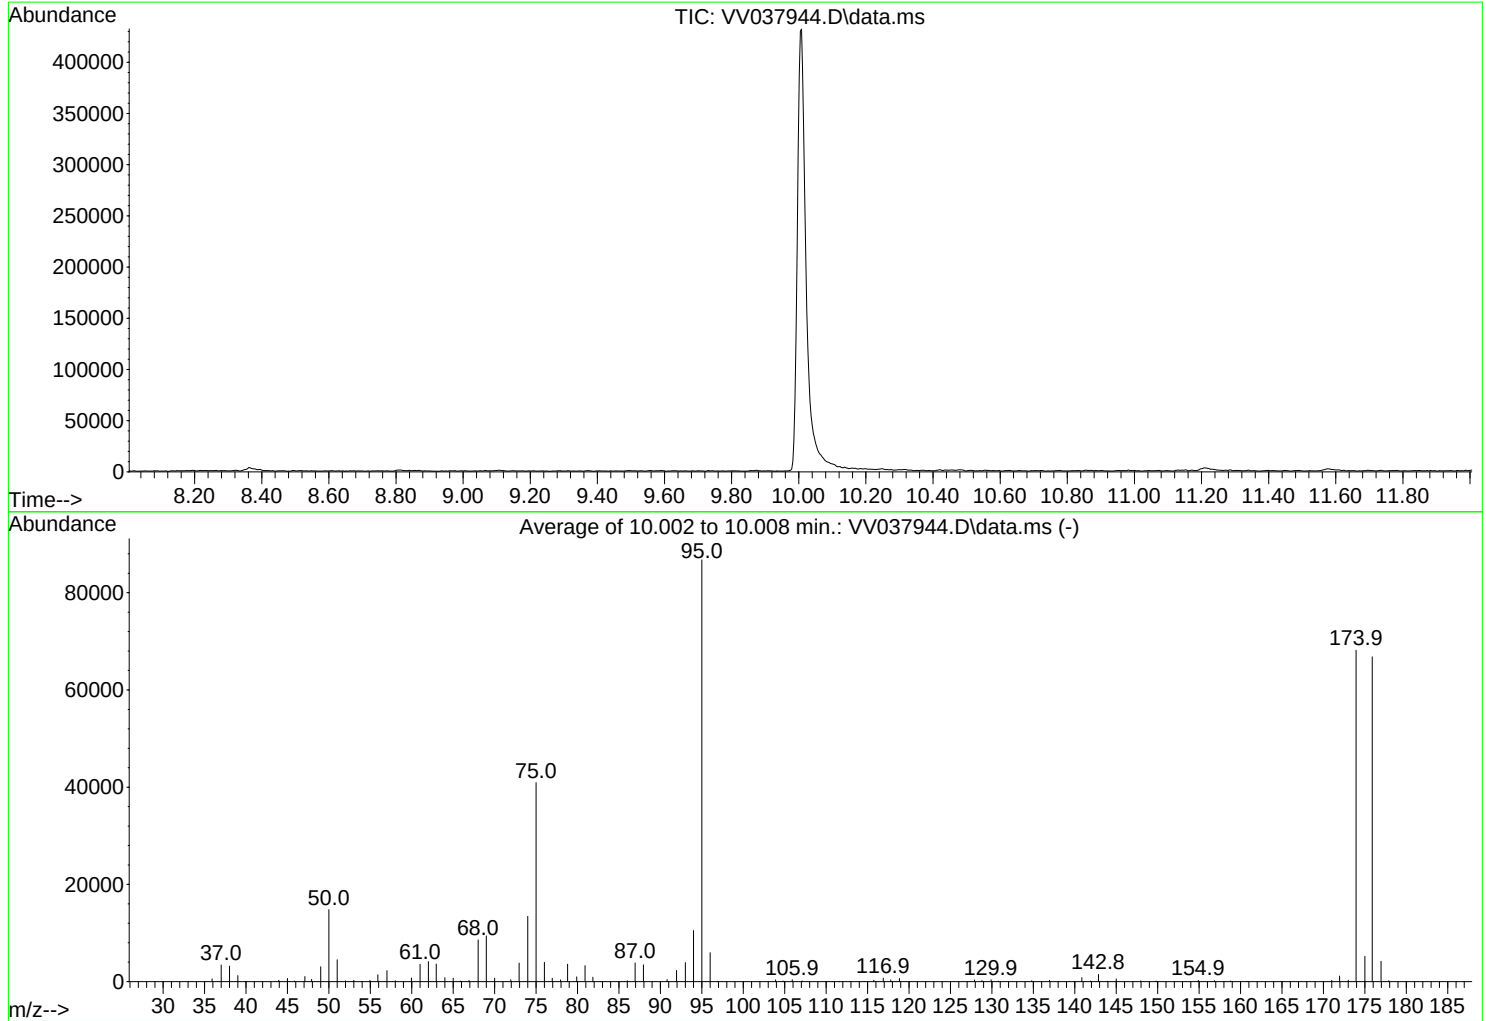

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	14799	PASS
75	95	30	80	47.2	40947	PASS
95	95	100	100	100.0	86765	PASS
96	95	5	9	6.9	5948	PASS
173	174	0.00	2	0.4	291	PASS
174	95	50	120	78.6	68176	PASS
175	174	5	9	7.6	5210	PASS
176	174	95	105	98.0	66821	PASS
177	176	5	10	6.2	4175	PASS

m/z	Abundance
40.00	311.0
44.00	650.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
35.90	578.0
37.00	3169.0
38.00	3169.0
39.00	1186.0
39.90	298.0
41.00	108.0
43.90	787.0
45.00	607.0
45.80	167.0
47.10	902.0
47.80	392.0
49.00	2882.0
50.00	13572.0
51.00	4444.0
52.00	152.0
53.00	287.0
53.90	114.0
54.90	268.0
55.90	1319.0
57.00	2100.0
58.00	186.0
60.00	773.0
61.00	3377.0
62.00	3983.0
63.00	3361.0
64.00	744.0
65.00	729.0
65.90	139.0
66.90	265.0
68.00	8296.0
69.00	8879.0
70.00	669.0
72.00	361.0
73.00	3695.0
74.00	12880.0
75.00	38296.0
76.00	3659.0
76.90	594.0
78.00	343.0
78.80	3476.0
79.90	849.0
80.90	3082.0
81.80	865.0
86.10	241.0
86.90	3444.0
87.90	3301.0
90.80	389.0
91.90	2223.0
93.00	3721.0
94.00	10057.0
95.00	81280.0
96.00	5814.0
104.00	334.0
104.80	107.0
105.90	364.0
107.10	162.0
111.60	109.0
115.70	280.0
116.90	679.0
117.80	328.0
118.80	680.0
127.90	320.0
128.80	217.0
129.90	340.0
130.80	133.0
134.90	178.0
136.90	203.0
140.80	724.0
141.90	130.0
142.90	1338.0
145.00	540.0
147.90	161.0
149.80	147.0
154.80	235.0
156.90	200.0
158.80	149.0
170.90	279.0
172.00	1099.0
173.00	873.0
174.00	61584.0
175.00	4701.0
175.90	60856.0
176.90	3952.0
177.90	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
35.90	597.0
37.00	3577.0
38.00	3268.0
39.00	1270.0
39.80	374.0
41.00	107.0
43.90	951.0
45.00	660.0
45.90	122.0
47.10	1110.0
47.90	466.0
49.00	3151.0
50.00	15325.0
51.00	4646.0
52.00	145.0
53.00	295.0
53.90	102.0
54.90	305.0
55.90	1506.0
57.00	2337.0
58.00	212.0
59.90	762.0
61.00	3630.0
62.00	4280.0
62.90	3758.0
64.00	882.0
65.00	757.0
65.90	157.0
66.90	260.0
68.00	8912.0
69.00	9897.0
70.00	763.0
71.90	355.0
73.00	3901.0
74.00	13708.0
75.00	42168.0
76.00	4146.0
77.00	737.0
77.90	349.0
78.80	3739.0
79.90	1018.0
80.90	3400.0
81.90	948.0
86.00	204.0
86.90	4008.0
87.90	3501.0
90.80	471.0
91.90	2354.0
93.00	4001.0
94.00	10785.0
95.00	89520.0
96.00	6086.0
103.90	350.0
104.80	148.0
105.90	407.0
107.10	167.0
111.60	105.0
112.90	106.0
115.70	304.0
116.90	779.0
117.80	391.0
118.90	684.0
127.90	405.0
128.80	242.0
129.90	443.0
130.80	127.0
134.80	169.0
137.00	265.0
140.80	848.0
141.90	164.0
142.90	1527.0
143.90	117.0
145.00	603.0
148.00	155.0
149.80	175.0
154.90	284.0
156.90	187.0
158.80	149.0
160.80	119.0
171.00	249.0
171.90	1206.0
173.90	70528.0
175.00	5441.0
175.90	69184.0
176.90	4246.0
177.90	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
35.90	546.0
37.00	3524.0
38.00	3117.0
39.00	1354.0
39.80	373.0
44.00	1095.0
45.00	676.0
45.90	122.0
47.10	1136.0
48.00	497.0
49.00	3146.0
50.00	15500.0
51.00	4466.0
52.00	209.0
53.00	229.0
55.00	263.0
55.90	1430.0
57.00	2415.0
58.00	168.0
59.90	718.0
61.00	3713.0
62.00	4087.0
62.90	3754.0
64.00	798.0
65.00	710.0
65.80	148.0
66.90	249.0
68.00	8544.0
69.00	9477.0
70.00	714.0
71.90	444.0
72.90	3840.0
74.00	13677.0
75.00	42376.0
76.00	4101.0
77.00	799.0
77.90	393.0
78.80	3593.0
79.90	1073.0
80.90	3402.0
81.90	973.0
82.80	110.0
85.90	192.0
87.00	4062.0
88.00	3555.0
90.80	461.0
92.00	2351.0
93.00	4029.0
94.00	10657.0
95.00	89496.0
96.00	5945.0
96.90	181.0
103.80	366.0
104.80	123.0
105.90	440.0
107.10	131.0
110.80	110.0
112.90	108.0
114.60	111.0
115.80	335.0
116.90	756.0
117.80	389.0
118.90	644.0
127.90	379.0
128.80	212.0
129.90	453.0
134.70	226.0
137.00	291.0
140.90	876.0
141.90	155.0
142.80	1619.0
143.90	144.0
145.00	541.0
148.00	150.0
149.80	128.0
155.00	291.0
156.80	172.0
158.80	104.0
160.80	117.0
171.10	260.0
171.90	1171.0
173.90	72416.0
175.00	5487.0
175.90	70424.0
177.00	4328.0
177.90	171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282