




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110824\
 Data File : VV037972.D
 Acq On : 08 Nov 2024 12:31
 Operator : SY/MD
 Sample : P4715-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL9

Manual IntegrationsAPPROVED

Quant Time: Nov 09 05:24:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 09 02:20:30 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/09/2024
 Supervised By :Mahesh Dadoda 11/11/2024

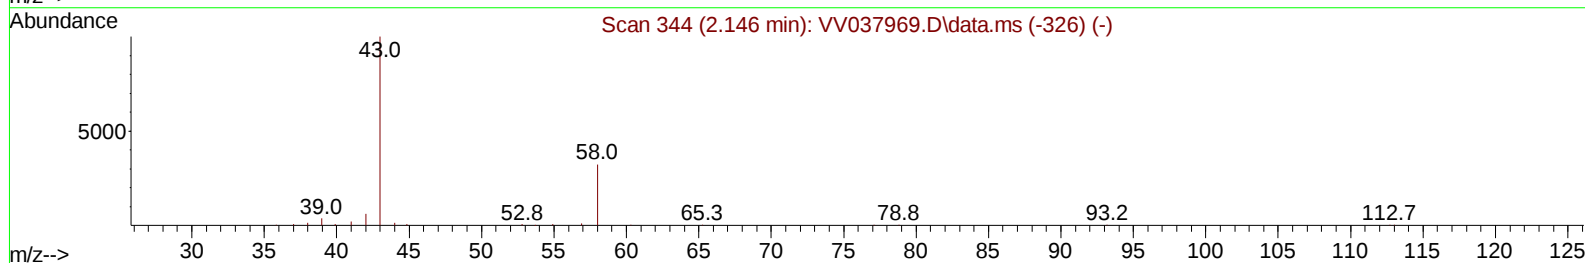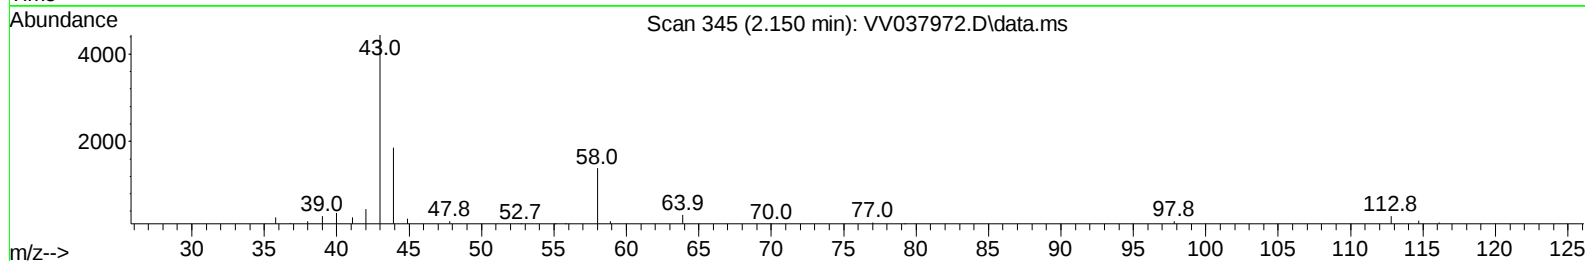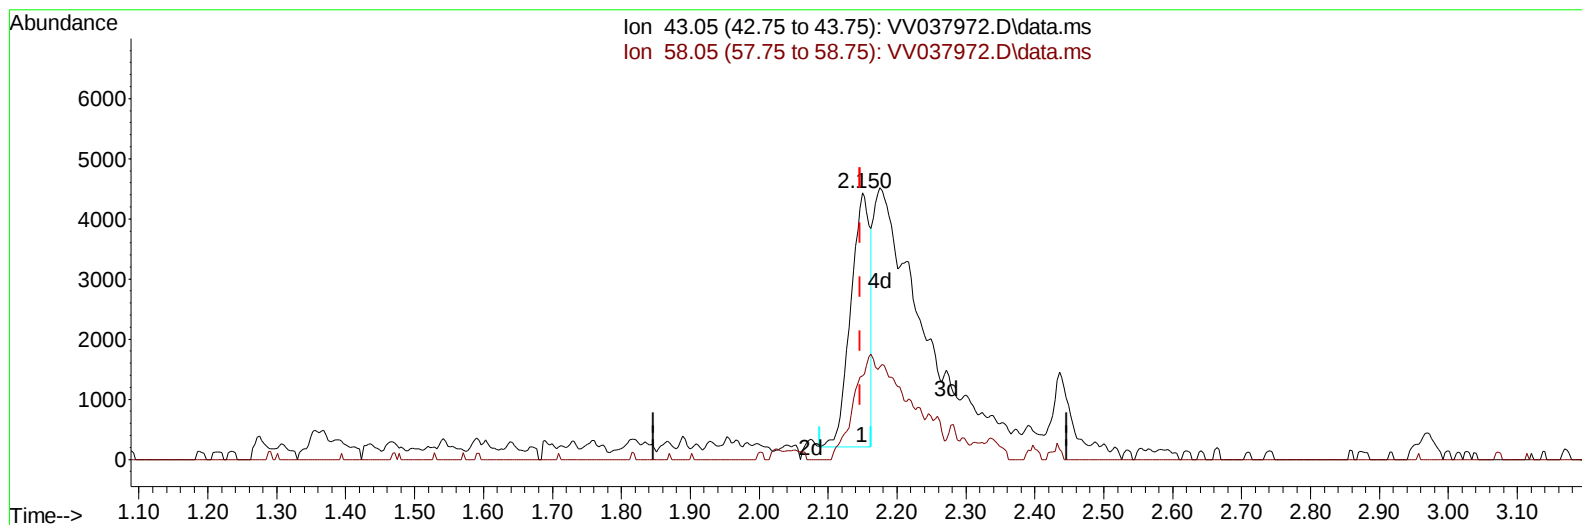

TIC: VV037972.D\data.ms

(13) Acetone (T)

2.150min (+ 0.003) 3.11 ug/L

response 8278

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.30	48.26
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110824\
Data File : VV037972.D
Acq On : 08 Nov 2024 12:31
Operator : SY/MD
Sample : P4715-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL9

Manual IntegrationsAPPROVED

Quant Time: Nov 09 05:24:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 09 02:20:30 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/09/2024
Supervised By :Mahesh Dadoda 11/11/2024

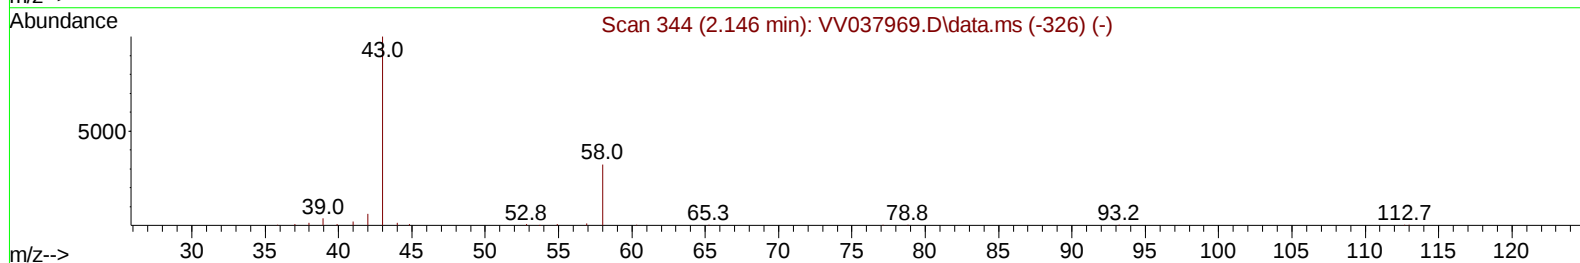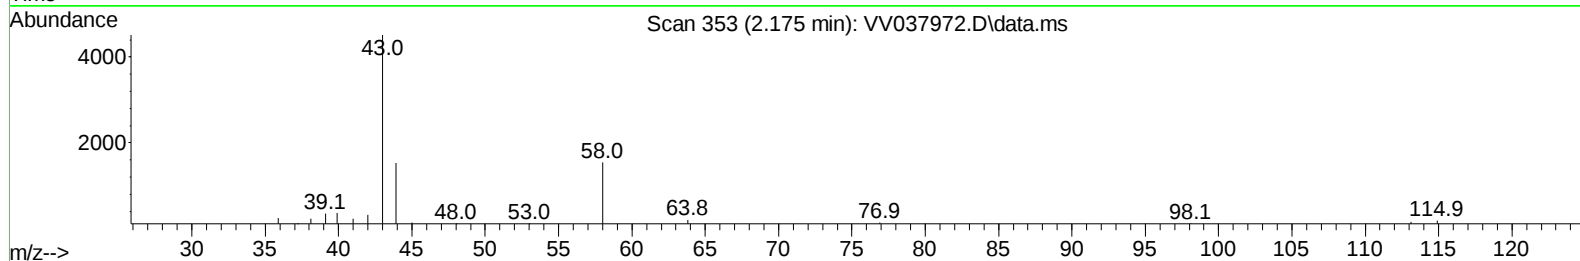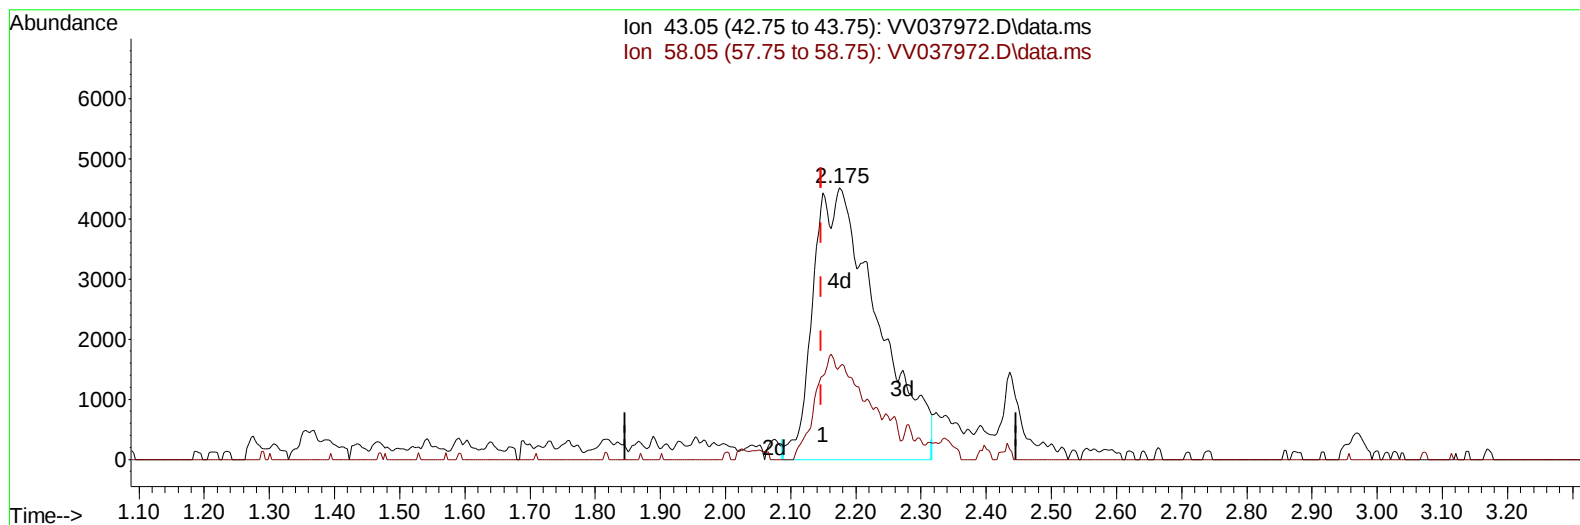

TIC: VV037972.D\data.ms

(13) Acetone (T)

2.175min (+ 0.029) 11.64 ug/L m

response 30995

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.30	12.89
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110824\
 Data File : VV037972.D
 Acq On : 08 Nov 2024 12:31
 Operator : SY/MD
 Sample : P4715-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAL9

Manual IntegrationsAPPROVED

Quant Time: Nov 09 05:24:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 09 02:20:30 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/09/2024
 Supervised By :Mahesh Dadoda 11/11/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.529	114		262931	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117		279998	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152		126099	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.275	65		90656	4.505	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.000%	
7) Chloroethane-d5	1.529	69		73190	4.462	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.200%	
11) 1,1-Dichloroethene-d2	2.053	65		40358	4.621	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.400%	
20) 2-Butanone-d5	3.844	46		170506	45.456	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.920%	
24) Chloroform-d	4.243	84		179928	4.905	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.000%	
26) 1,2-Dichloroethane-d4	4.940	65		87979	5.366	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.400%	
32) Benzene-d6	4.953	84		340233	4.712	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.200%	
36) 1,2-Dichloropropane-d6	5.985	67		106763	5.063	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.200%	
41) Toluene-d8	7.239	98		281961	4.345	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.800%	
43) trans-1,3-Dichloroprop...	7.558	79		29999	3.679	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.600%	
46) 2-Hexanone-d5	8.030	63		160291	50.588	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.180%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84		89592	5.270	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.400%	
66) 1,2-Dichlorobenzene-d4	11.554	152		110182	5.298	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.000%	
Target Compounds							
13) Acetone	2.175	43		30995m	11.641	ug/L	
16) Methylene chloride	2.439	84		446210	21.282	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110824\
Data File : VV037972.D
Acq On : 08 Nov 2024 12:31
Operator : SY/MD
Sample : P4715-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL9

Manual IntegrationsAPPROVED

Quant Time: Nov 09 05:24:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 09 02:20:30 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 11/09/2024
Supervised By :Mahesh Dadoda 11/11/2024

