
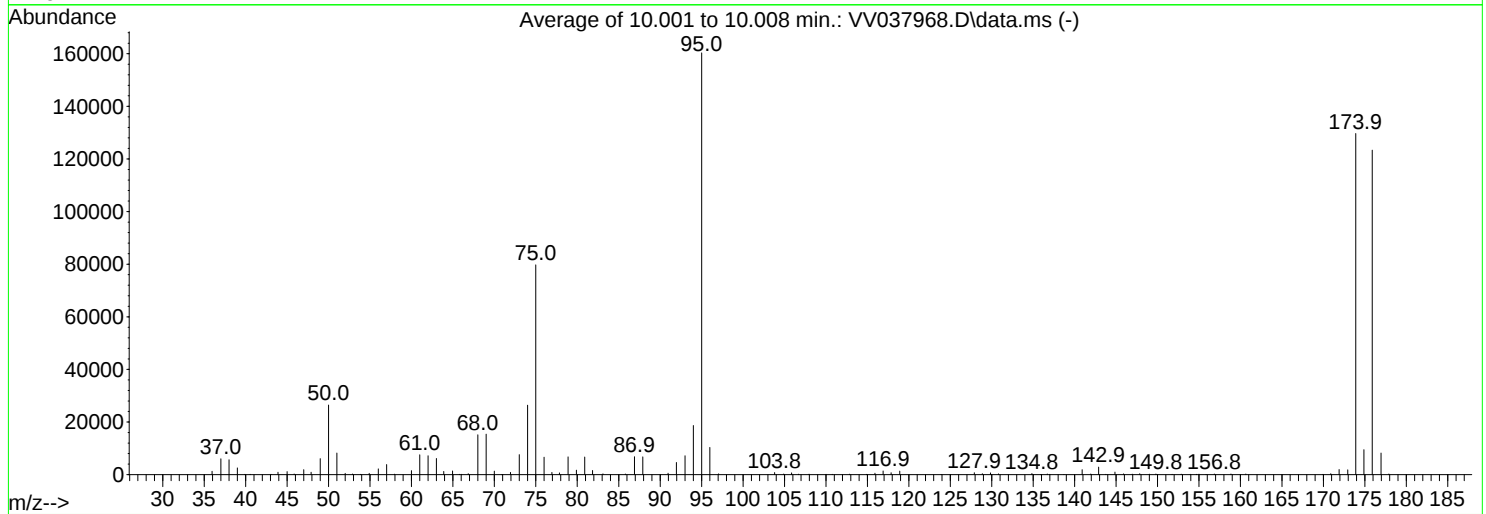


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV110824\
Data File : VV037968.D
Acq On : 08 Nov 2024 08:55
Operator : SY/MD
Sample : BFB283
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB283

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Nov 09 02:20:30 2024

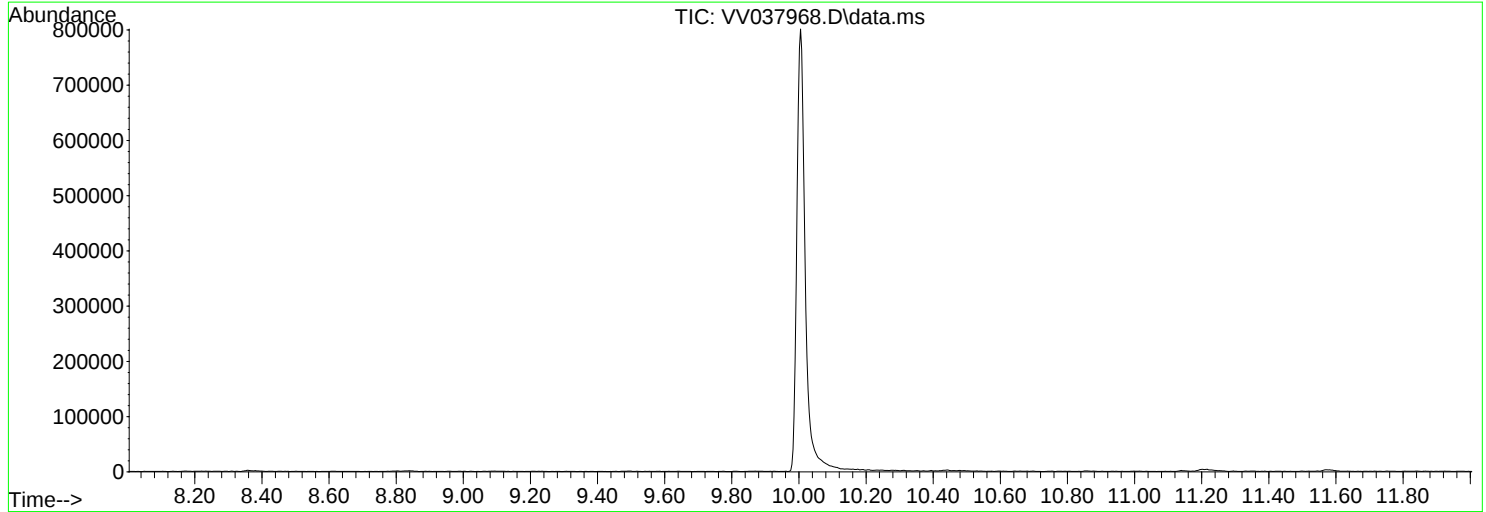

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	26456	PASS
75	95	30	80	49.7	79760	PASS
95	95	100	100	100.0	160341	PASS
96	95	5	9	6.5	10364	PASS
173	174	0.00	2	1.4	1835	PASS
174	95	50	120	80.9	129691	PASS
175	174	5	9	7.3	9514	PASS
176	174	95	105	95.1	123360	PASS
177	176	5	10	6.6	8200	PASS

m/z	Abundance
39.80	284.0
43.80	432.0
57.00	131.0
77.00	114.0
77.20	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
35.90	1366.0
37.00	6090.0
38.00	5668.0
39.00	2585.0
40.00	384.0
40.50	148.0
43.10	105.0
44.00	1382.0
45.00	1158.0
45.90	259.0
46.90	1842.0
47.90	955.0
49.00	6096.0
50.00	26576.0
51.00	8438.0
52.00	466.0
52.90	183.0
54.80	482.0
56.00	2093.0
57.00	3741.0
57.90	165.0
60.00	1623.0
61.00	7392.0
62.00	6718.0
63.00	6508.0
63.90	1167.0
64.90	1355.0
65.80	180.0
66.10	150.0
66.80	344.0
68.00	15350.0
69.00	15467.0
70.00	1349.0
72.00	765.0
73.00	7349.0
74.00	26048.0
75.00	79984.0
76.00	6924.0
77.00	903.0
77.90	774.0
78.90	6923.0
79.90	1683.0
80.90	6654.0
81.90	1421.0
83.10	284.0
85.80	267.0
86.90	6715.0
87.90	6656.0
90.90	462.0
91.90	4557.0
93.00	6831.0
94.00	19128.0
95.00	159232.0
96.00	10524.0
97.10	383.0
103.80	743.0
105.00	226.0
105.90	767.0
106.70	195.0
108.00	104.0
109.90	122.0
110.80	123.0
112.80	234.0
114.90	160.0
115.90	594.0
116.90	1328.0
117.90	775.0
118.90	1256.0
123.90	107.0
127.90	745.0
128.90	384.0
129.80	748.0
130.80	348.0
134.90	477.0
136.70	188.0
137.00	230.0
140.90	1974.0
141.90	269.0
142.90	2700.0
143.80	160.0
144.90	1019.0
145.90	375.0
146.90	156.0
147.80	401.0
149.00	224.0
149.80	150.0
151.90	117.0
152.80	138.0
154.00	121.0
154.70	291.0
156.80	317.0
158.90	235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

160.60	232.0
170.00	104.0
170.90	365.0
171.90	1881.0
173.00	1737.0
173.90	125080.0
174.90	9047.0
175.90	118920.0
177.00	8182.0
177.90	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
36.00	1332.0
37.00	6233.0
38.00	5806.0
39.00	2620.0
40.00	410.0
40.60	146.0
43.10	124.0
43.90	1384.0
45.00	1171.0
45.90	251.0
47.00	1945.0
47.90	933.0
49.00	6262.0
50.00	27176.0
51.00	8348.0
51.90	489.0
52.90	300.0
53.90	141.0
54.90	476.0
56.00	2212.0
57.00	4129.0
58.00	150.0
60.00	1596.0
61.00	7790.0
62.00	7347.0
63.00	6311.0
63.90	1250.0
65.00	1475.0
65.80	169.0
66.80	344.0
68.00	15662.0
69.00	15890.0
70.00	1374.0
71.90	857.0
73.00	7927.0
74.00	27184.0
75.00	82432.0
76.00	6838.0
76.90	1032.0
77.80	663.0
78.90	6960.0
79.90	1730.0
80.90	6833.0
81.90	1629.0
83.10	324.0
85.80	284.0
86.90	7016.0
87.90	7020.0
90.90	586.0
91.90	4717.0
93.00	7420.0
94.00	19240.0
95.00	165312.0
96.00	10812.0
97.10	314.0
103.80	818.0
104.90	248.0
105.80	696.0
106.70	166.0
107.90	166.0
110.00	131.0
110.70	113.0
112.90	189.0
114.90	157.0
115.90	596.0
116.90	1387.0
117.80	793.0
118.90	1370.0
123.90	116.0
127.90	721.0
128.90	398.0
129.80	692.0
130.80	356.0
134.80	477.0
136.70	231.0
137.00	216.0
140.90	1932.0
142.00	217.0
142.90	2926.0
143.70	144.0
144.90	980.0
145.90	362.0
147.00	188.0
147.90	389.0
149.00	228.0
149.80	235.0
151.70	104.0
152.90	226.0
154.00	132.0
155.00	316.0
155.80	100.0
156.80	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

158.90	214.0
160.60	244.0
169.90	132.0
170.90	405.0
171.90	1986.0
172.90	1856.0
173.90	133888.0
174.90	9735.0
175.90	127320.0
176.90	8534.0
177.90	251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
36.00	1159.0
37.00	5779.0
38.00	5529.0
39.00	2397.0
40.00	377.0
43.00	119.0
43.90	1315.0
45.00	1111.0
45.80	284.0
47.10	1881.0
47.90	839.0
49.00	5837.0
50.00	25616.0
51.00	7804.0
52.10	457.0
52.90	332.0
53.80	205.0
55.00	494.0
56.00	2233.0
57.00	3953.0
58.00	176.0
60.00	1399.0
61.00	7377.0
62.00	7492.0
63.00	5690.0
63.90	1242.0
65.00	1454.0
66.00	138.0
66.90	394.0
68.00	14522.0
69.00	14755.0
70.00	1275.0
70.90	114.0
71.90	870.0
73.00	7603.0
74.00	25912.0
75.00	76864.0
76.00	6183.0
76.90	1058.0
77.80	615.0
78.90	6414.0
79.90	1675.0
80.90	6579.0
81.80	1635.0
83.10	260.0
85.80	249.0
86.90	6747.0
87.90	6582.0
91.00	685.0
92.00	4609.0
93.00	7275.0
94.00	17672.0
95.00	156480.0
96.00	9756.0
97.00	270.0
103.80	812.0
104.80	275.0
105.80	608.0
106.70	138.0
107.90	223.0
110.10	115.0
110.70	140.0
112.90	151.0
114.90	140.0
115.90	506.0
116.90	1433.0
117.80	706.0
118.90	1382.0
127.90	652.0
128.80	341.0
129.90	552.0
130.80	269.0
134.80	379.0
135.90	111.0
136.70	274.0
138.70	129.0
140.90	1764.0
142.00	203.0
142.90	2974.0
144.80	929.0
145.90	286.0
147.00	176.0
147.90	354.0
149.00	155.0
149.80	301.0
151.60	115.0
152.90	241.0
153.90	122.0
155.00	287.0
155.90	101.0
156.90	232.0
158.70	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

160.70	193.0
169.90	140.0
170.90	387.0
171.90	1958.0
172.90	1911.0
173.90	130104.0
174.90	9759.0
175.90	123840.0
176.90	7884.0
177.90	269.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283