




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
 Data File : VV038008.D
 Acq On : 11 Nov 2024 20:06
 Operator : SY/MD
 Sample : P4749-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GCP90

Manual IntegrationsAPPROVED

Quant Time: Nov 12 04:44:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 12 04:39:46 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/12/2024
 Supervised By :Semsettin Yesilyurt 11/12/2024

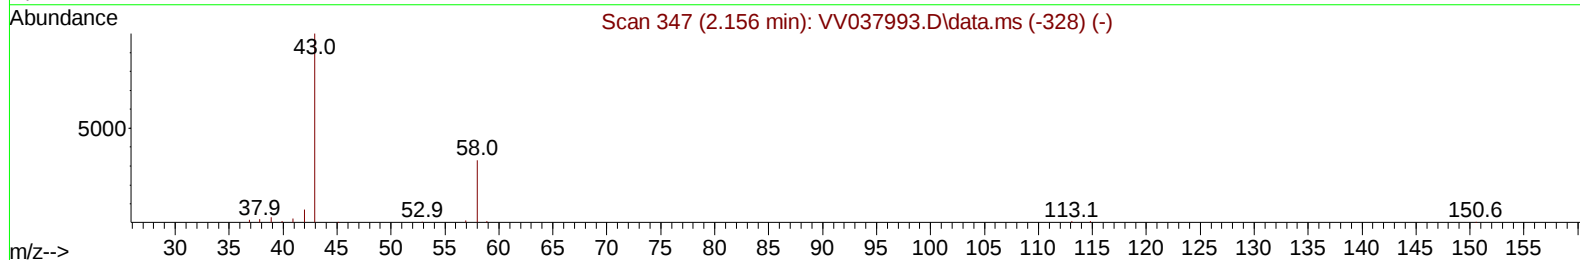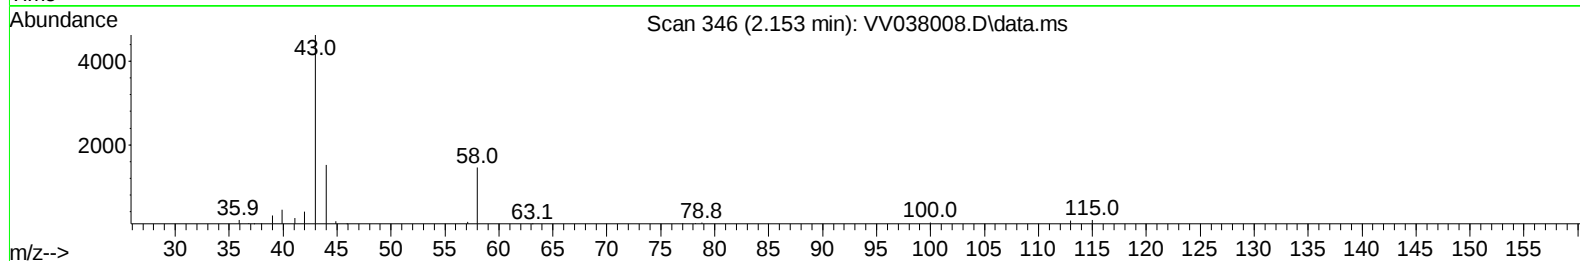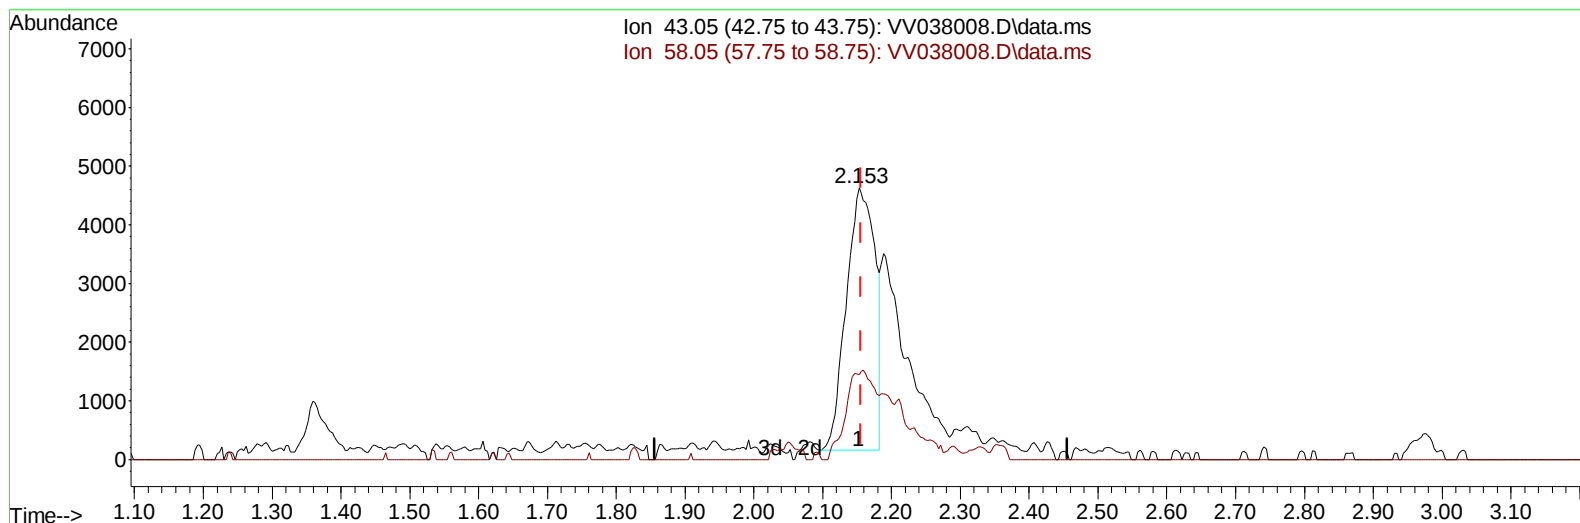

TIC: VV038008.D\data.ms

(13) Acetone (T)

2.153min (-0.003) 4.80 ug/L

response 12903

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.30	34.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
 Data File : VV038008.D
 Acq On : 11 Nov 2024 20:06
 Operator : SY/MD
 Sample : P4749-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GCP90

Manual IntegrationsAPPROVED

Quant Time: Nov 12 04:44:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 12 04:39:46 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/12/2024
 Supervised By :Semsettin Yesilyurt 11/12/2024

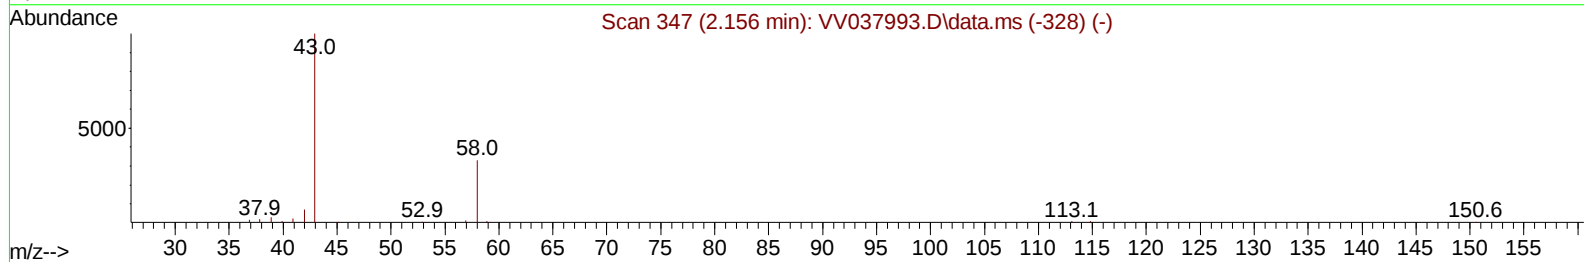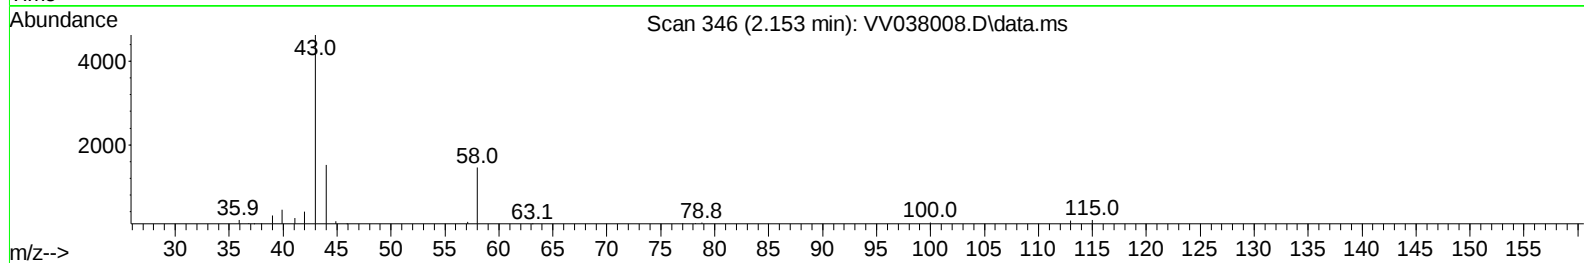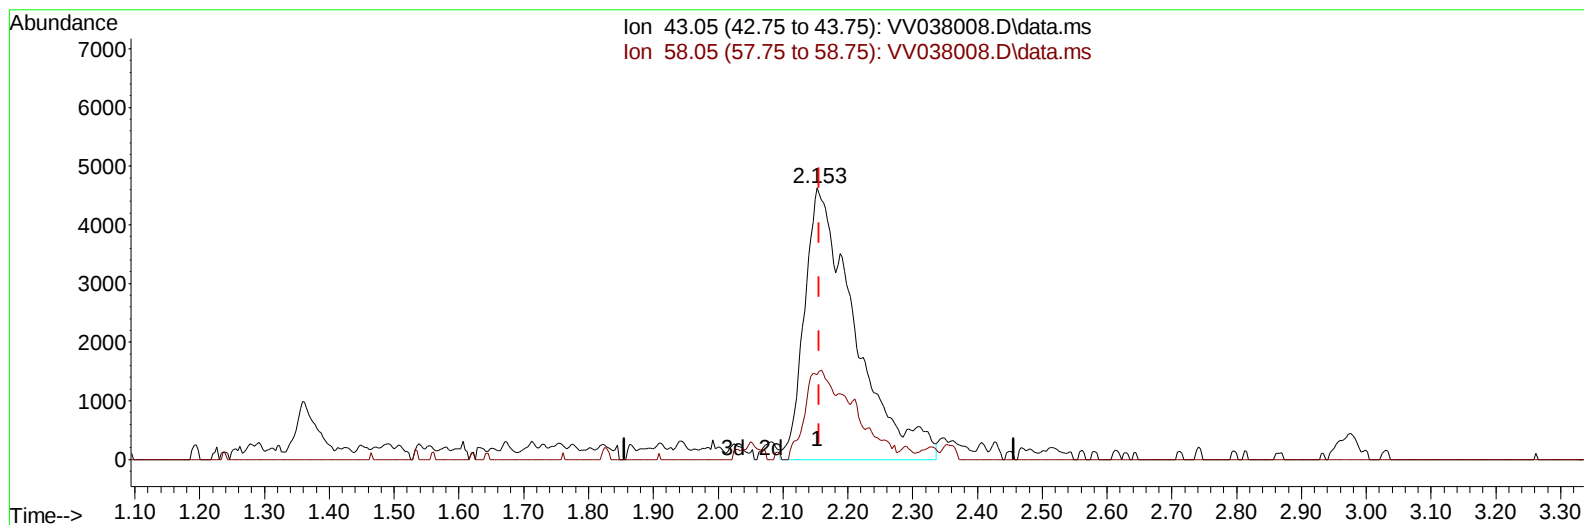

TIC: VV038008.D\data.ms

(13) Acetone (T)

2.153min (-0.003) 9.32 ug/L m

response 25034

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.30	17.82
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
 Data File : VV038008.D
 Acq On : 11 Nov 2024 20:06
 Operator : SY/MD
 Sample : P4749-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GCP90

Manual IntegrationsAPPROVED

Quant Time: Nov 12 04:44:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 12 04:39:46 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/12/2024
 Supervised By :Semsettin Yesilyurt 11/12/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.529	114		265192	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117		278706	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152		128568	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.275	65		80915	3.986	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.800%	
7) Chloroethane-d5	1.529	69		69976	4.230	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.600%	
11) 1,1-Dichloroethene-d2	2.053	65		37196	4.223	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.400%	
20) 2-Butanone-d5	3.831	46		176223	46.580	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.160%	
24) Chloroform-d	4.243	84		164794	4.454	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%	
26) 1,2-Dichloroethane-d4	4.940	65		80559	4.872	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.400%	
32) Benzene-d6	4.953	84		312833	4.352	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.000%	
36) 1,2-Dichloropropane-d6	5.985	67		100173	4.773	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.400%	
41) Toluene-d8	7.239	98		263773	4.083	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.600%	
43) trans-1,3-Dichloroprop...	7.558	79		31437	3.873	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.400%	
46) 2-Hexanone-d5	8.024	63		151410	48.006	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.020%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84		86045	5.085	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.600%	
66) 1,2-Dichlorobenzene-d4	11.554	152		104676	4.936	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.800%	
Target Compounds							
13) Acetone	2.153	43		25034m	9.322	ug/L	
34) Trichloroethene	5.828	95		152375	7.185	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
Data File : VV038008.D
Acq On : 11 Nov 2024 20:06
Operator : SY/MD
Sample : P4749-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GCP90

Manual IntegrationsAPPROVED

Quant Time: Nov 12 04:44:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 12 04:39:46 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/12/2024
Supervised By :Semsettin Yesilyurt 11/12/2024

