

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
 Data File : VV038000.D
 Acq On : 11 Nov 2024 16:53
 Operator : SY/MD
 Sample : P4749-18DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GCP91DL

Quant Time: Nov 12 04:42:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 12 04:39:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	285063	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	297363	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	137027	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	84787	3.886	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.800%
7) Chloroethane-d5	1.529	69	70184	3.947	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.000%
11) 1,1-Dichloroethene-d2	2.044	65	39614	4.184	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.600%
20) 2-Butanone-d5	3.828	46	170947	42.035	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.080%
24) Chloroform-d	4.240	84	178628	4.491	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%
26) 1,2-Dichloroethane-d4	4.937	65	84266	4.741	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
32) Benzene-d6	4.950	84	334140	4.357	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
36) 1,2-Dichloropropane-d6	5.982	67	107173	4.786	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.800%
41) Toluene-d8	7.239	98	289706	4.204	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.000%
43) trans-1,3-Dichloroprop...	7.558	79	39442	4.555	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.000%
46) 2-Hexanone-d5	8.037	63	148842	44.231	ug/L	0.01
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.460%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	87124	4.825	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.600%
66) 1,2-Dichlorobenzene-d4	11.554	152	111599	4.938	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.800%
Target Compounds					Qvalue	
34) Trichloroethene	5.825	95	128248	5.668	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
Data File : VV038000.D
Acq On : 11 Nov 2024 16:53
Operator : SY/MD
Sample : P4749-18DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GCP91DL


Quant Time: Nov 12 04:42:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 12 04:39:46 2024
Response via : Initial Calibration

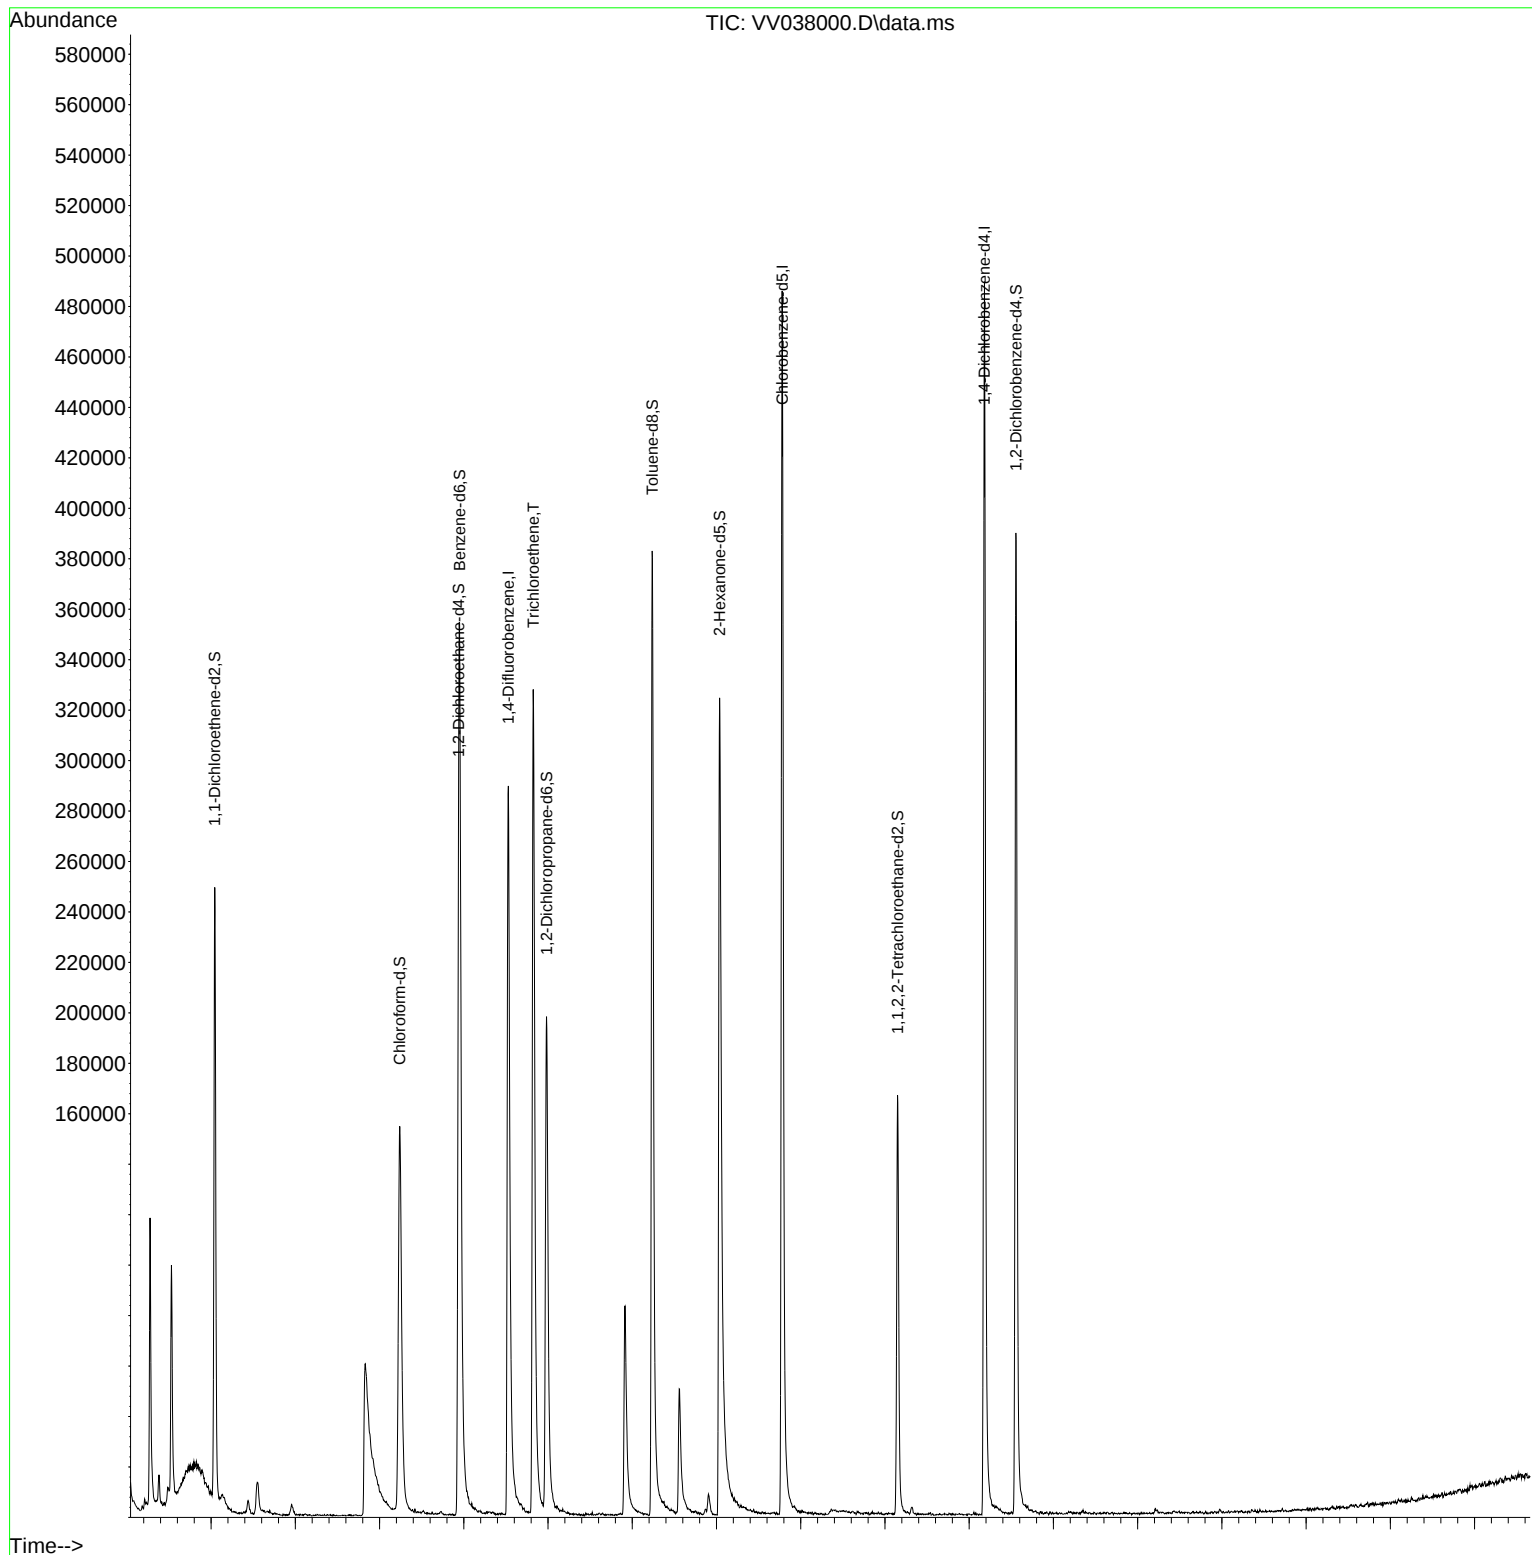

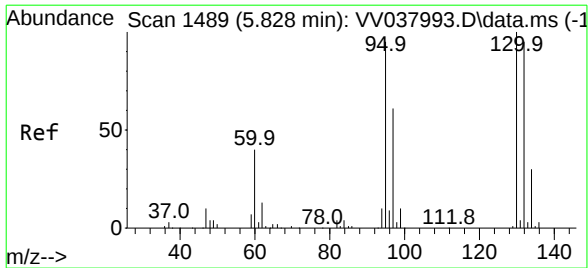

#34
 Trichloroethene
 Concen: 5.668 ug/L
 RT: 5.825 min Scan# 14
 Delta R.T. -0.003 min
 Lab File: VV038000.D
 Acq: 11 Nov 2024 16:53

Instrument :
 MSVOA_V
 ClientSampleId :
 GCP91DL

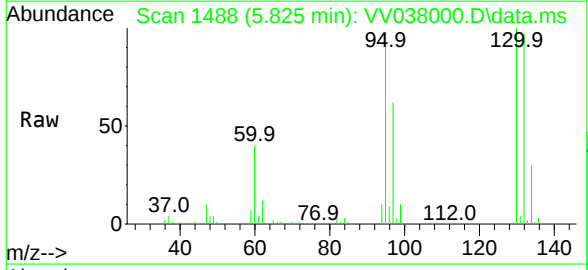

Tgt Ion:	95	Resp:	128248
Ion	Ratio	Lower	Upper
95	100		
97	62.7	46.9	87.1
132	98.3	70.5	130.9
130	101.6	72.9	135.3

