

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
 Data File : VV038002.D
 Acq On : 11 Nov 2024 17:41
 Operator : SY/MD
 Sample : P4749-13DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GCP86DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	94	rBV	115224	143512	14.62%	1.635%
2	1.529	145	152	166	rVB	94407	122762	12.51%	1.398%
3	2.047	303	313	330	rVB	251981	372505	37.96%	4.243%
4	2.548	455	469	483	rBV	21099	49685	5.06%	0.566%
5	2.953	582	595	608	rBV2	29038	58334	5.94%	0.664%
6	3.834	852	869	906	rBV	63945	354797	36.16%	4.041%
7	4.240	980	995	1026	rVB	153464	414983	42.29%	4.727%
8	4.947	1203	1215	1249	rBV2	369295	956546	97.48%	10.895%
9	5.529	1386	1396	1428	rBV	243310	554376	56.49%	6.314%
10	5.825	1472	1488	1522	rBV	388619	835987	85.19%	9.522%
11	5.982	1526	1537	1565	rVV	197310	437998	44.64%	4.989%
12	6.911	1814	1826	1852	rBV2	87401	195794	19.95%	2.230%
13	7.236	1917	1927	1952	rBV	399802	758471	77.29%	8.639%
14	7.558	2017	2027	2046	rBV2	52739	114413	11.66%	1.303%
15	7.905	2126	2135	2148	rVB3	18165	31756	3.24%	0.362%
16	8.037	2166	2176	2220	rBV	359355	981286	100.00%	11.177%
17	8.780	2397	2407	2437	rBV	403603	728959	74.29%	8.303%
18	10.149	2823	2833	2850	rBV	186123	316528	32.26%	3.605%
19	11.181	3144	3154	3178	rBV	377155	655848	66.84%	7.470%
20	11.554	3257	3270	3293	rBV	407743	695142	70.84%	7.918%

Sum of corrected areas: 8779682




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
Data File : VV038002.D
Acq On : 11 Nov 2024 17:41
Operator : SY/MD
Sample : P4749-13DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GCP86DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

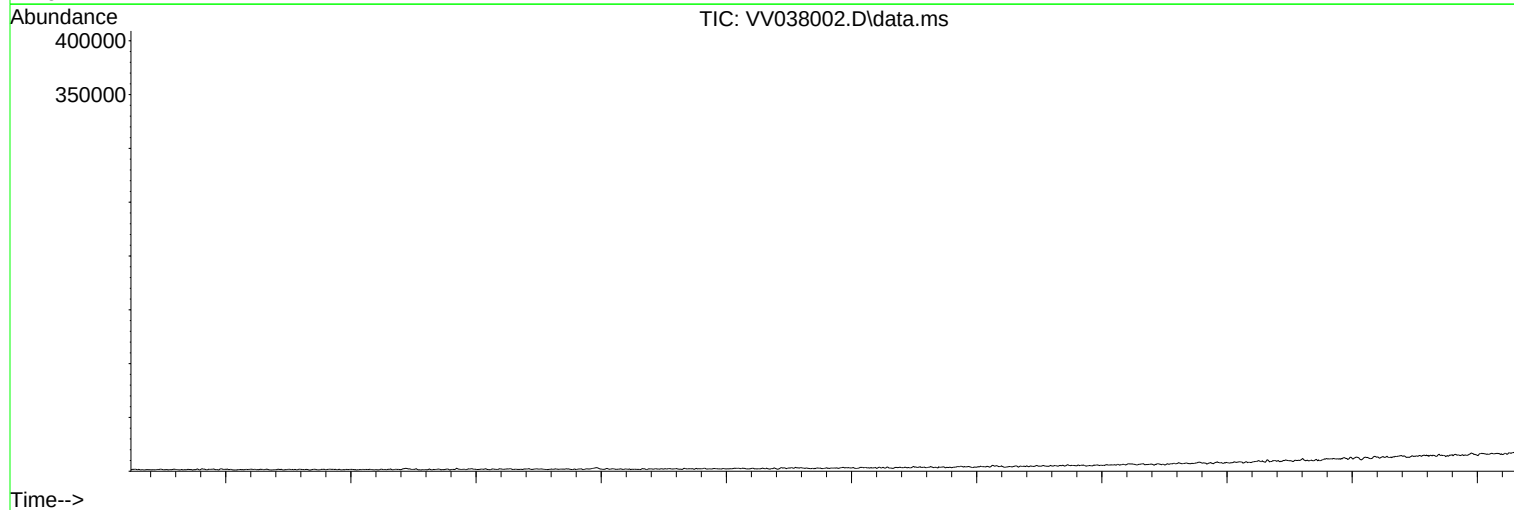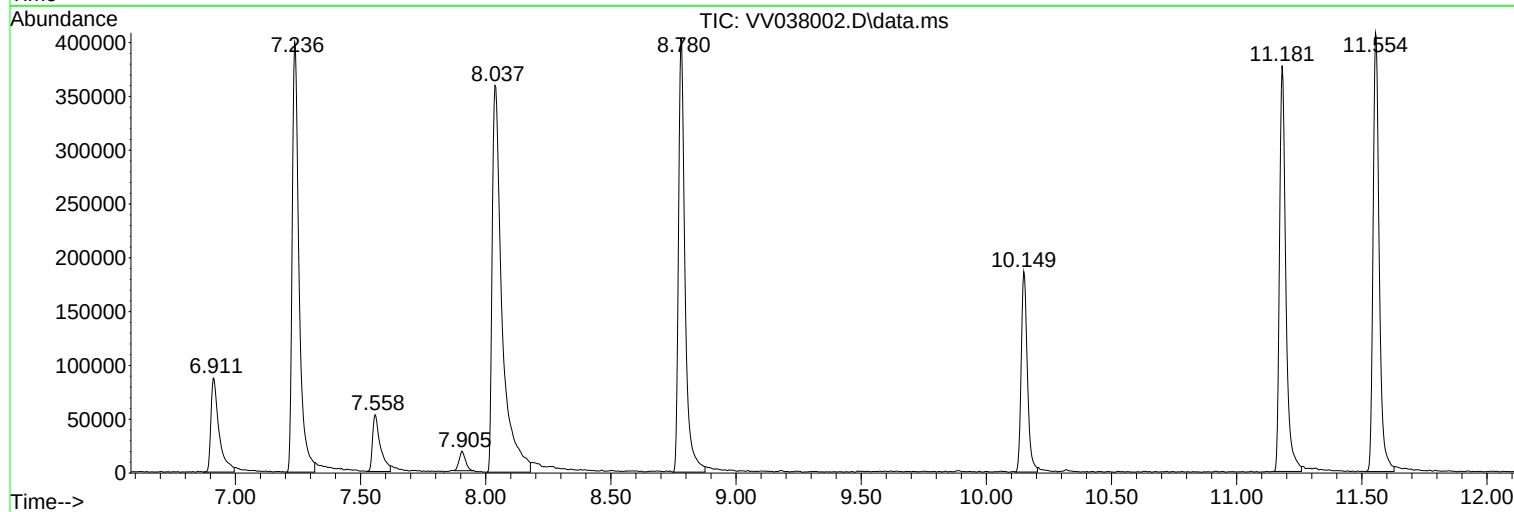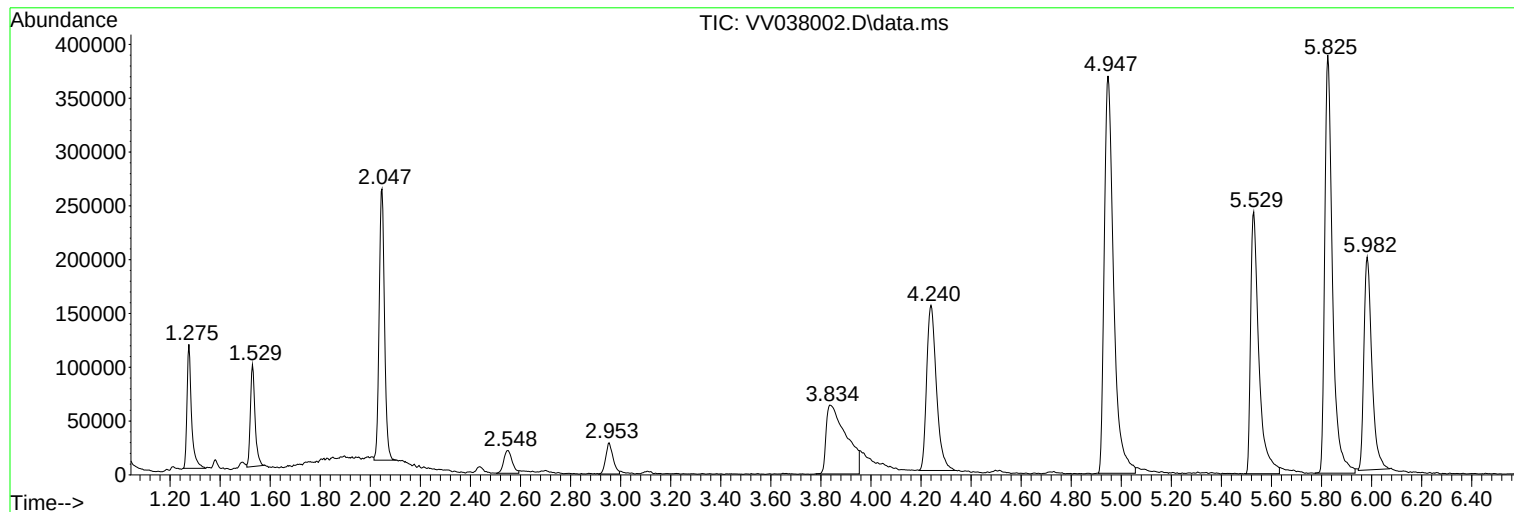

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
Data File : VV038002.D
Acq On : 11 Nov 2024 17:41
Operator : SY/MD
Sample : P4749-13DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GCP86DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
Data File : VV038002.D
Acq On : 11 Nov 2024 17:41
Operator : SY/MD
Sample : P4749-13DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GCP86DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
