
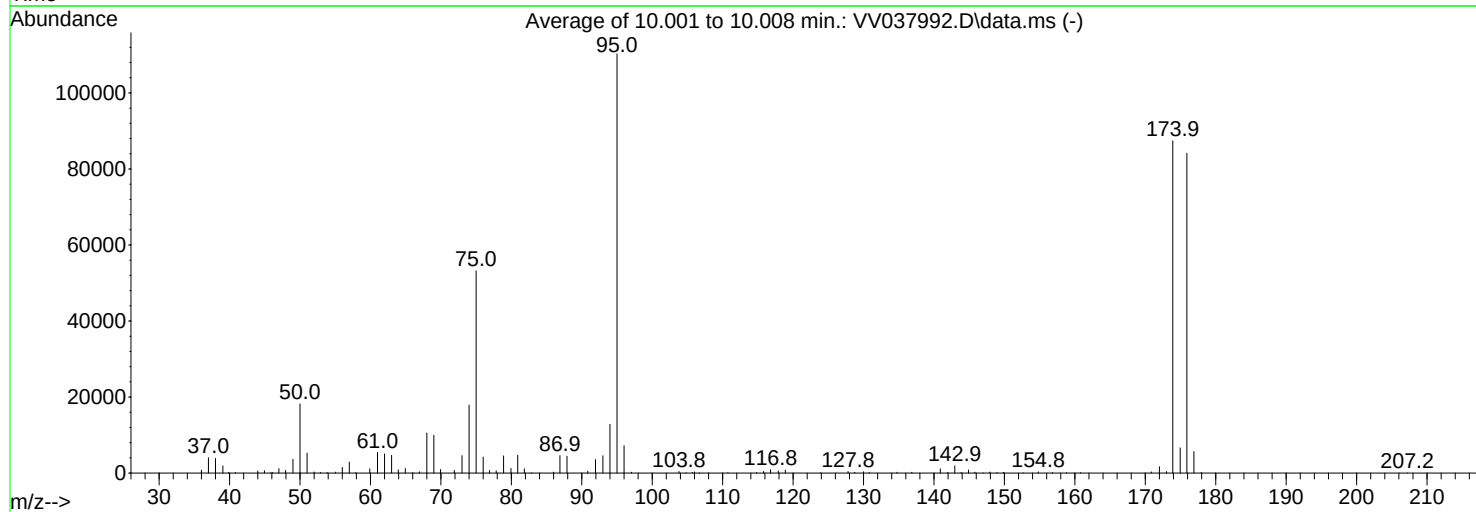


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111124\
Data File : VV037992.D
Acq On : 11 Nov 2024 10:41
Operator : SY/MD
Sample : BFB284
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB284

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Nov 12 04:39:46 2024

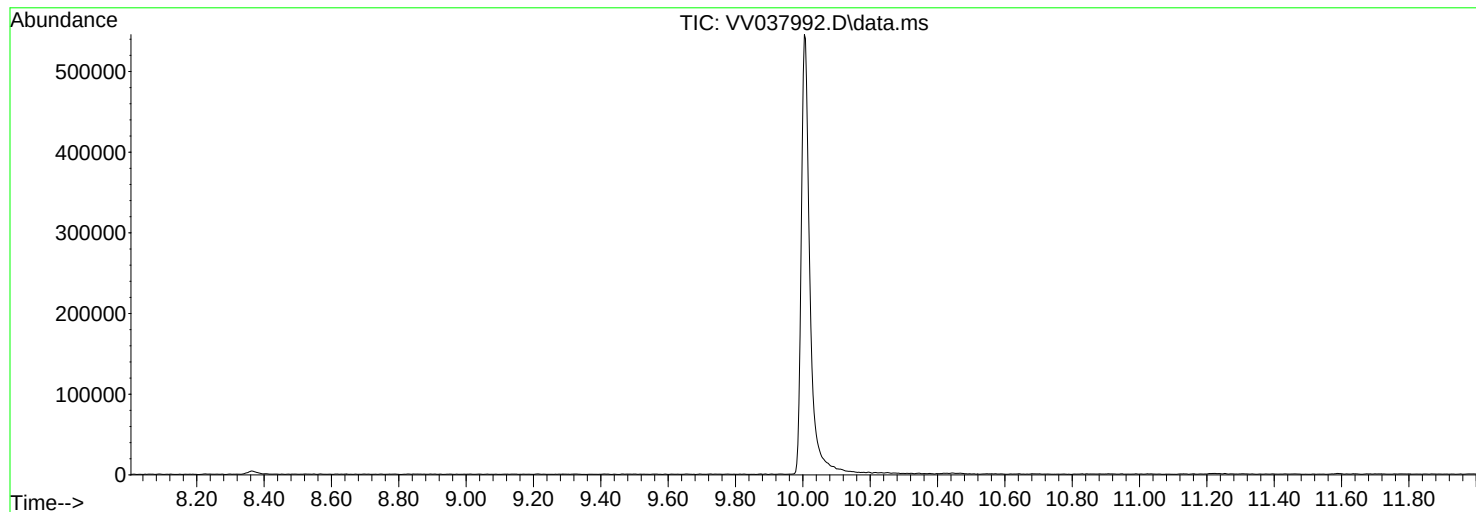

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	18192	PASS
75	95	30	80	48.2	53219	PASS
95	95	100	100	100.0	110317	PASS
96	95	5	9	6.5	7219	PASS
173	174	0.00	2	0.5	406	PASS
174	95	50	120	79.2	87403	PASS
175	174	5	9	7.6	6636	PASS
176	174	95	105	96.3	84157	PASS
177	176	5	10	6.7	5678	PASS

m/z	Abundance
39.90	272.0
44.00	541.0
76.90	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
36.00	825.0
37.00	3990.0
38.00	3750.0
39.00	1689.0
39.80	420.0
40.80	162.0
44.00	1082.0
44.90	568.0
45.90	141.0
46.10	141.0
47.00	1003.0
48.00	702.0
49.00	3674.0
50.00	17392.0
51.00	5282.0
52.00	251.0
52.90	146.0
53.80	125.0
55.00	248.0
56.00	1332.0
57.00	2681.0
59.90	1041.0
61.00	5525.0
62.00	4910.0
63.00	4411.0
64.00	805.0
65.00	1192.0
66.00	146.0
67.00	287.0
68.00	10110.0
69.00	9535.0
69.90	841.0
71.90	616.0
73.00	4064.0
74.00	17208.0
75.00	50920.0
76.00	4050.0
76.90	798.0
77.90	589.0
78.90	4266.0
79.90	1173.0
80.90	4581.0
81.90	1174.0
86.00	199.0
86.90	4517.0
87.90	4230.0
90.90	498.0
92.00	3323.0
93.00	4294.0
94.00	12319.0
95.00	104824.0
96.00	6757.0
97.10	204.0
103.80	424.0
106.00	454.0
110.70	109.0
114.80	154.0
115.80	415.0
116.80	837.0
117.90	514.0
118.90	769.0
127.80	425.0
128.80	193.0
130.00	293.0
130.80	141.0
134.80	254.0
136.80	207.0
140.90	1107.0
142.00	145.0
143.00	1725.0
143.80	143.0
144.90	740.0
145.90	292.0
148.00	234.0
149.00	112.0
149.80	122.0
152.70	107.0
154.80	272.0
158.70	116.0
170.80	337.0
172.00	1575.0
173.90	80816.0
175.00	5714.0
175.90	77600.0
176.90	5643.0
178.00	110.0
207.20	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

m/z	Abundance
36.00	818.0
37.00	4112.0
38.00	3922.0
39.10	1975.0
39.90	410.0
40.90	185.0
44.00	1118.0
44.90	644.0
45.80	153.0
46.20	150.0
47.00	1281.0
47.90	744.0
49.00	3774.0
50.00	18912.0
51.00	5398.0
52.00	303.0
52.90	164.0
53.80	156.0
55.10	269.0
56.00	1535.0
57.00	2957.0
57.90	114.0
59.90	1167.0
61.00	5619.0
62.00	5206.0
63.00	4871.0
64.00	907.0
65.00	1263.0
66.00	116.0
67.00	366.0
68.00	10886.0
69.00	10236.0
70.00	953.0
71.90	756.0
73.00	4757.0
74.00	18600.0
75.00	55160.0
76.00	4353.0
76.90	838.0
77.80	627.0
78.90	4737.0
79.90	1230.0
80.90	4938.0
81.90	1192.0
82.90	120.0
86.00	257.0
86.90	4726.0
87.90	4507.0
90.90	516.0
91.90	3676.0
93.00	4702.0
94.00	13300.0
95.00	113800.0
96.00	7421.0
97.10	257.0
103.80	420.0
104.80	105.0
106.00	475.0
106.70	114.0
110.70	103.0
114.80	164.0
115.80	464.0
116.80	902.0
117.90	573.0
118.90	815.0
123.90	107.0
127.80	450.0
128.70	218.0
130.00	369.0
130.80	178.0
134.70	252.0
136.80	233.0
140.90	1158.0
142.00	195.0
142.90	2008.0
143.80	164.0
144.90	835.0
145.80	223.0
147.00	102.0
148.00	291.0
148.90	151.0
149.80	199.0
154.80	321.0
156.80	213.0
158.80	143.0
160.80	169.0
170.80	348.0
172.00	1778.0
173.90	90704.0
174.90	6848.0
175.90	86792.0
176.90	5828.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284

177.90

161.0

Instrument :

MSVOA_V

ClientSampleId :

BFB284

m/z	Abundance
36.00	699.0
37.00	3990.0
38.00	3849.0
39.10	2080.0
39.90	388.0
40.90	141.0
44.00	1102.0
45.00	702.0
46.00	168.0
47.00	1250.0
47.90	609.0
49.00	3453.0
50.00	18272.0
51.00	5095.0
52.00	315.0
52.90	158.0
53.90	146.0
55.00	253.0
56.00	1617.0
57.00	3002.0
57.90	130.0
59.90	1121.0
61.00	5146.0
62.00	5022.0
63.00	4736.0
63.90	923.0
64.90	1185.0
66.90	406.0
68.00	10651.0
69.00	10135.0
70.00	1034.0
71.90	816.0
73.00	4988.0
74.00	17968.0
75.00	53576.0
76.00	4256.0
77.00	786.0
77.80	578.0
78.90	4596.0
80.00	1314.0
80.90	4522.0
81.80	1001.0
82.90	113.0
86.00	306.0
86.90	4574.0
87.90	4556.0
90.80	491.0
91.90	3738.0
93.00	4693.0
94.00	12851.0
95.00	112328.0
96.00	7478.0
97.00	258.0
103.80	409.0
104.80	162.0
105.70	476.0
106.70	122.0
108.00	101.0
110.80	114.0
114.80	146.0
115.80	444.0
116.80	914.0
117.90	555.0
118.90	730.0
127.80	431.0
128.80	228.0
130.00	418.0
130.80	227.0
134.70	199.0
136.90	219.0
140.90	1133.0
141.90	171.0
142.90	2008.0
143.90	138.0
144.90	838.0
145.70	197.0
147.90	311.0
148.90	171.0
149.90	215.0
154.80	323.0
156.80	295.0
158.90	163.0
160.80	212.0
170.90	287.0
172.00	1684.0
173.00	1217.0
173.90	90688.0
175.00	7347.0
175.90	88080.0
176.90	5562.0
177.90	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB284