
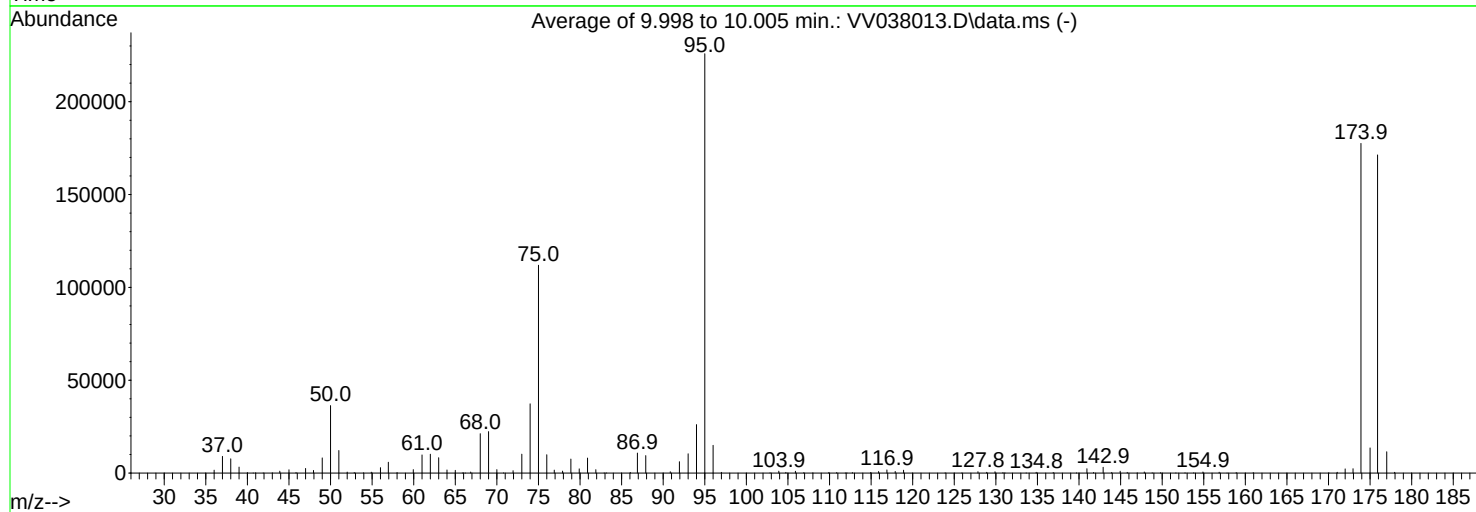


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111224\
Data File : VV038013.D
Acq On : 12 Nov 2024 11:29
Operator : SY/MD
Sample : BFB285
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB285

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Nov 13 00:39:48 2024

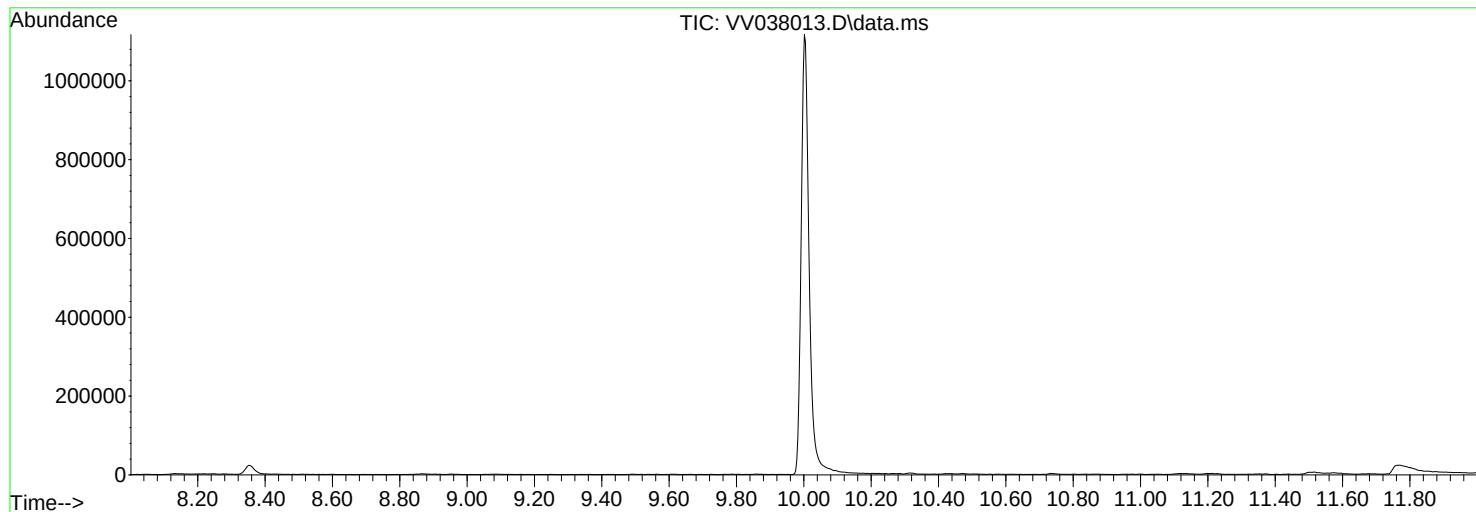

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	36344	PASS
75	95	30	80	49.6	111933	PASS
95	95	100	100	100.0	225835	PASS
96	95	5	9	6.6	14957	PASS
173	174	0.00	2	1.3	2351	PASS
174	95	50	120	78.6	177536	PASS
175	174	5	9	7.6	13555	PASS
176	174	95	105	96.5	171328	PASS
177	176	5	10	6.7	11475	PASS

Scan 2774 (9.960 min): VV038013.D\data.ms
BFB285

m/z	Abundance
40.00	234.0
43.10	138.0
43.90	462.0
55.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
36.00	1634.0
37.00	8621.0
38.00	7568.0
39.00	3176.0
40.00	462.0
40.70	126.0
41.90	124.0
43.00	208.0
43.90	1331.0
45.00	1626.0
45.90	255.0
47.00	2619.0
47.90	1443.0
49.00	7591.0
50.00	34696.0
51.00	12100.0
52.00	496.0
52.80	297.0
54.00	125.0
54.90	622.0
56.00	2849.0
56.90	5459.0
58.00	256.0
59.90	1897.0
61.00	9388.0
62.00	9522.0
63.00	7792.0
64.00	1674.0
65.00	1400.0
65.80	115.0
66.20	138.0
66.90	580.0
68.00	20056.0
69.00	21536.0
70.00	1933.0
70.80	103.0
71.90	1362.0
73.00	9803.0
74.00	35528.0
75.00	107608.0
76.00	9737.0
76.90	1549.0
77.90	935.0
78.90	7020.0
79.90	2177.0
80.90	7576.0
81.90	1810.0
83.20	127.0
86.00	264.0
86.90	10144.0
87.90	9309.0
90.80	625.0
91.90	5714.0
93.00	10163.0
94.00	24784.0
95.00	214848.0
96.00	14787.0
97.00	343.0
102.90	163.0
103.90	955.0
104.70	376.0
105.90	862.0
106.90	219.0
109.90	263.0
110.80	223.0
111.90	123.0
112.70	255.0
115.00	287.0
115.90	794.0
116.90	1593.0
117.80	809.0
118.90	1335.0
127.90	745.0
128.80	487.0
129.90	697.0
130.80	250.0
131.10	248.0
134.80	397.0
136.90	309.0
139.60	119.0
141.00	2248.0
141.80	301.0
142.90	3161.0
143.90	268.0
145.00	975.0
145.80	374.0
147.80	593.0
148.70	146.0
149.80	253.0
151.70	101.0
152.80	140.0
153.80	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

154.90	510.0
157.00	423.0
158.90	334.0
161.00	246.0
170.00	133.0
171.00	504.0
172.00	2365.0
172.90	2135.0
173.90	162560.0
175.00	12472.0
175.90	157440.0
177.00	10823.0
177.90	377.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
36.00	1632.0
37.00	9354.0
38.00	8024.0
39.00	3318.0
40.00	464.0
41.00	122.0
43.00	220.0
44.00	1493.0
45.00	1858.0
45.80	318.0
47.00	2548.0
48.00	1548.0
49.00	8430.0
50.00	37672.0
51.00	12661.0
52.00	562.0
52.90	286.0
54.00	117.0
54.90	591.0
56.00	3035.0
57.00	6081.0
58.00	268.0
60.00	1904.0
61.00	10152.0
62.00	10616.0
63.00	8567.0
64.00	1769.0
65.00	1510.0
65.90	150.0
66.90	610.0
68.00	22152.0
69.00	23216.0
70.00	1958.0
70.80	137.0
72.00	1320.0
73.00	10640.0
74.00	38728.0
75.00	116232.0
76.00	10074.0
76.90	1625.0
77.90	1150.0
78.90	7837.0
79.90	2358.0
80.90	8445.0
81.90	1897.0
83.20	124.0
86.00	294.0
86.90	11268.0
87.90	9695.0
90.80	779.0
92.00	6401.0
93.00	10750.0
94.00	27088.0
95.00	233856.0
96.00	15564.0
97.00	394.0
102.90	145.0
103.90	1067.0
104.80	388.0
105.90	1046.0
106.90	217.0
108.00	111.0
109.90	266.0
110.80	278.0
112.10	123.0
112.70	275.0
115.00	335.0
115.90	876.0
116.90	1810.0
117.90	907.0
118.90	1638.0
123.90	138.0
127.80	755.0
128.90	398.0
129.90	729.0
130.90	266.0
133.60	105.0
134.90	419.0
136.90	333.0
139.70	112.0
140.90	2423.0
141.70	373.0
142.90	3305.0
143.90	260.0
144.90	1000.0
145.80	382.0
147.00	107.0
147.90	607.0
148.80	160.0
149.80	221.0
151.70	107.0
152.70	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

153.80	181.0
154.90	607.0
156.80	492.0
158.90	302.0
161.00	253.0
170.10	102.0
171.00	463.0
172.00	2299.0
172.90	2388.0
173.90	183808.0
175.00	14093.0
175.90	178112.0
177.00	11996.0
178.00	436.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

m/z	Abundance
36.00	1470.0
37.00	9059.0
38.00	7485.0
39.00	3245.0
40.00	445.0
41.00	184.0
42.90	231.0
44.00	1654.0
45.00	1844.0
45.90	339.0
47.00	2316.0
47.90	1284.0
49.00	8524.0
50.00	36664.0
51.00	11683.0
52.00	589.0
52.90	266.0
53.90	106.0
54.90	570.0
56.00	2891.0
57.00	6001.0
58.00	230.0
60.00	1836.0
61.00	9814.0
62.00	10351.0
63.00	8474.0
64.00	1612.0
65.00	1520.0
66.00	145.0
66.80	517.0
68.00	21448.0
69.00	22240.0
70.00	1687.0
70.80	111.0
72.00	1234.0
73.00	10098.0
74.00	37656.0
75.00	111960.0
76.00	9852.0
76.90	1614.0
77.90	1152.0
78.90	7812.0
79.90	2265.0
80.90	8285.0
81.90	1785.0
82.90	162.0
86.10	374.0
86.90	10910.0
87.90	9252.0
90.90	807.0
92.00	6286.0
93.00	10276.0
94.00	26496.0
95.00	228800.0
96.00	14520.0
97.00	425.0
102.80	125.0
103.90	1067.0
104.80	382.0
105.90	1085.0
106.90	210.0
108.00	173.0
109.90	180.0
110.90	294.0
112.10	161.0
112.80	238.0
114.90	359.0
115.90	857.0
116.90	1717.0
118.00	902.0
118.90	1727.0
123.90	157.0
125.90	107.0
127.80	752.0
129.00	355.0
129.90	779.0
130.90	235.0
133.70	112.0
134.90	444.0
136.90	368.0
139.80	109.0
140.90	2379.0
141.70	348.0
142.90	2934.0
143.90	242.0
144.90	1031.0
145.80	392.0
147.00	150.0
147.90	579.0
148.90	167.0
149.80	135.0
151.60	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285

152.70	188.0
153.80	206.0
154.90	647.0
156.80	507.0
157.80	115.0
158.80	209.0
160.90	197.0
171.10	378.0
172.00	2058.0
173.00	2531.0
173.90	186240.0
175.00	14101.0
175.90	178432.0
177.00	11605.0
178.00	434.0

Instrument :
MSVOA_V
ClientSampleId :
BFB285