




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038043.D
Acq On : 13 Nov 2024 14:08
Operator : SY/MD
Sample : P4761-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AL6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 11/14/2024
Supervised By :Mahesh Dadoda 11/18/2024

Quant Time: Nov 13 23:11:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 13 00:39:48 2024
Response via : Initial Calibration

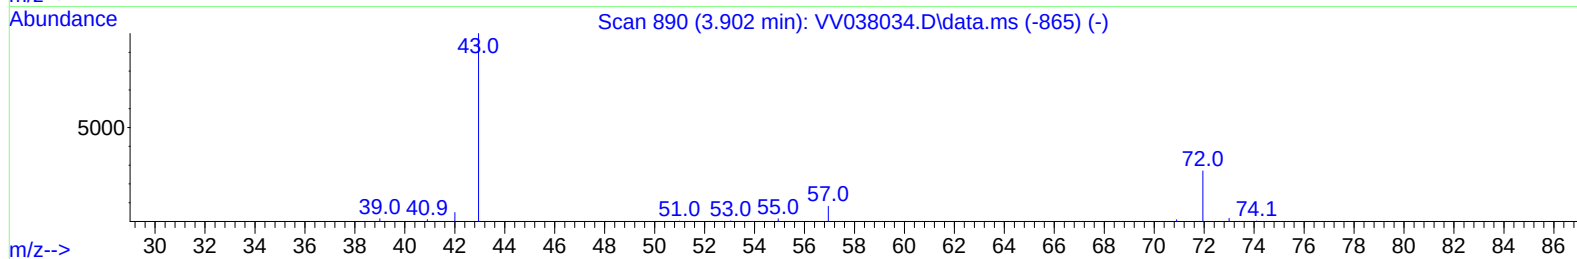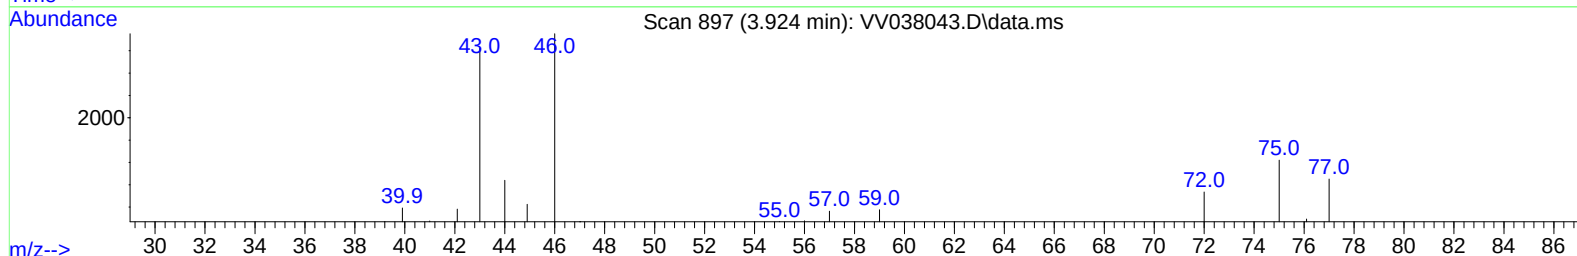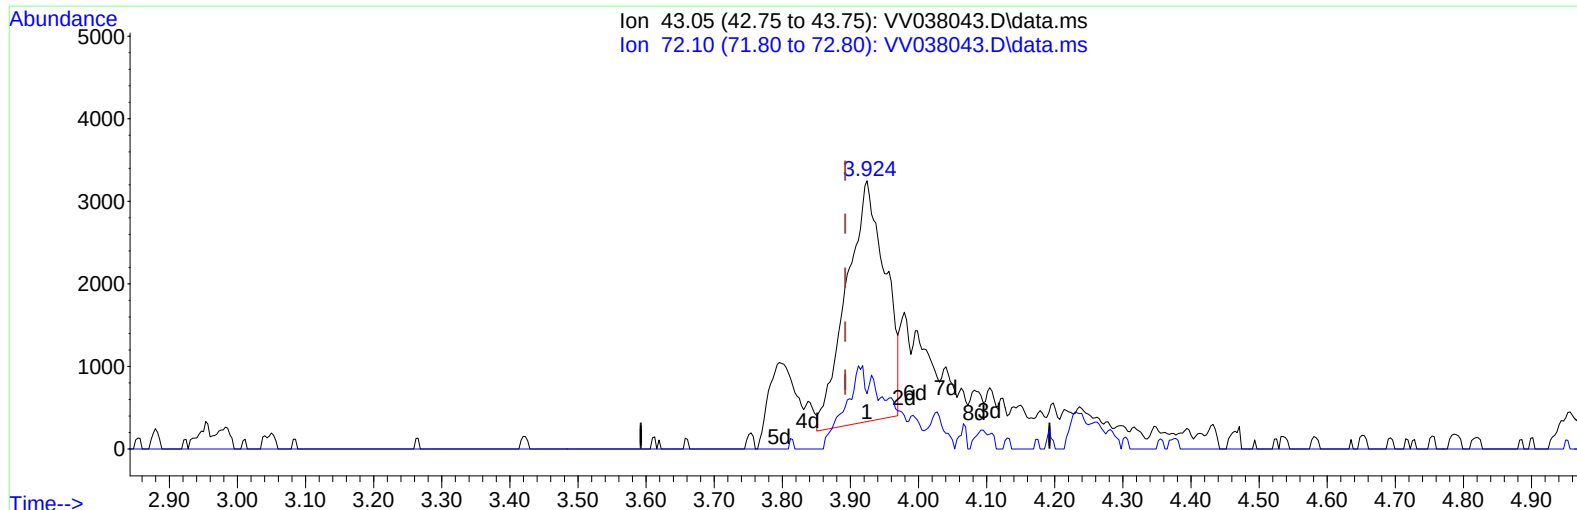

TIC: VV038043.D\data.ms

(21) 2-Butanone (T)

3.924min (+ 0.032) 3.21 ug/L

response 11483

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	28.40	18.58
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038043.D
Acq On : 13 Nov 2024 14:08
Operator : SY/MD
Sample : P4761-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AL6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 11/14/2024
Supervised By :Mahesh Dadoda 11/18/2024

Quant Time: Nov 13 23:11:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 13 00:39:48 2024
Response via : Initial Calibration

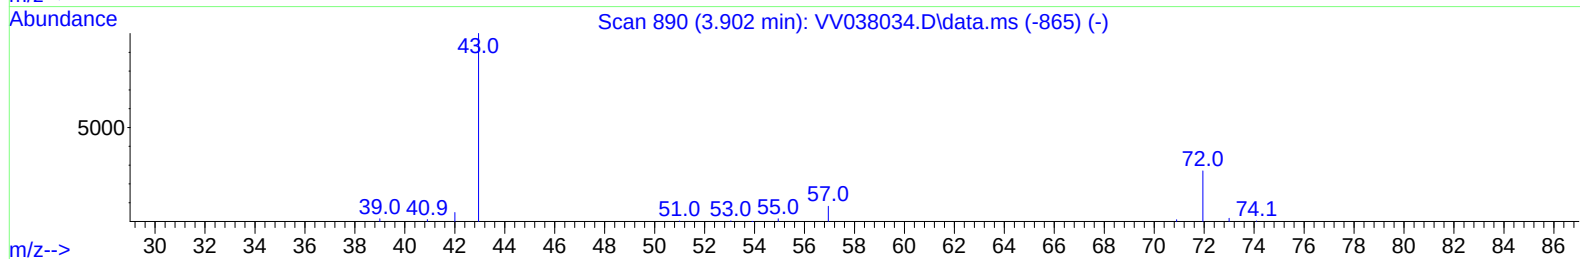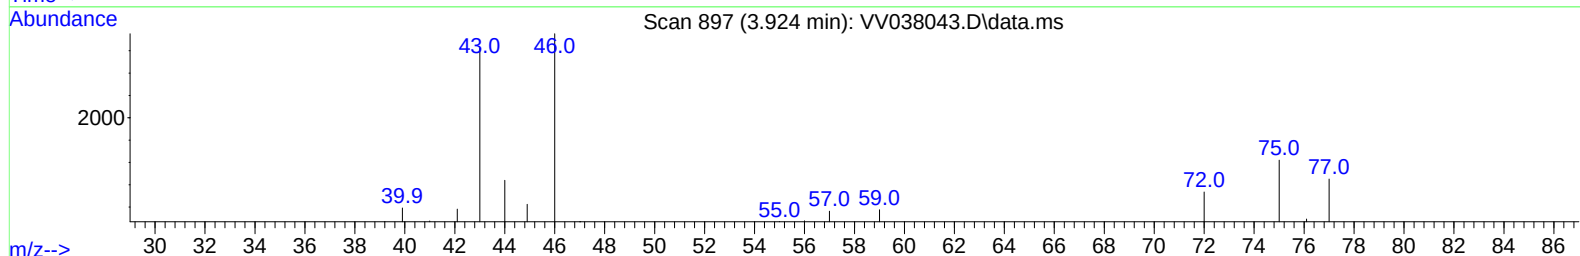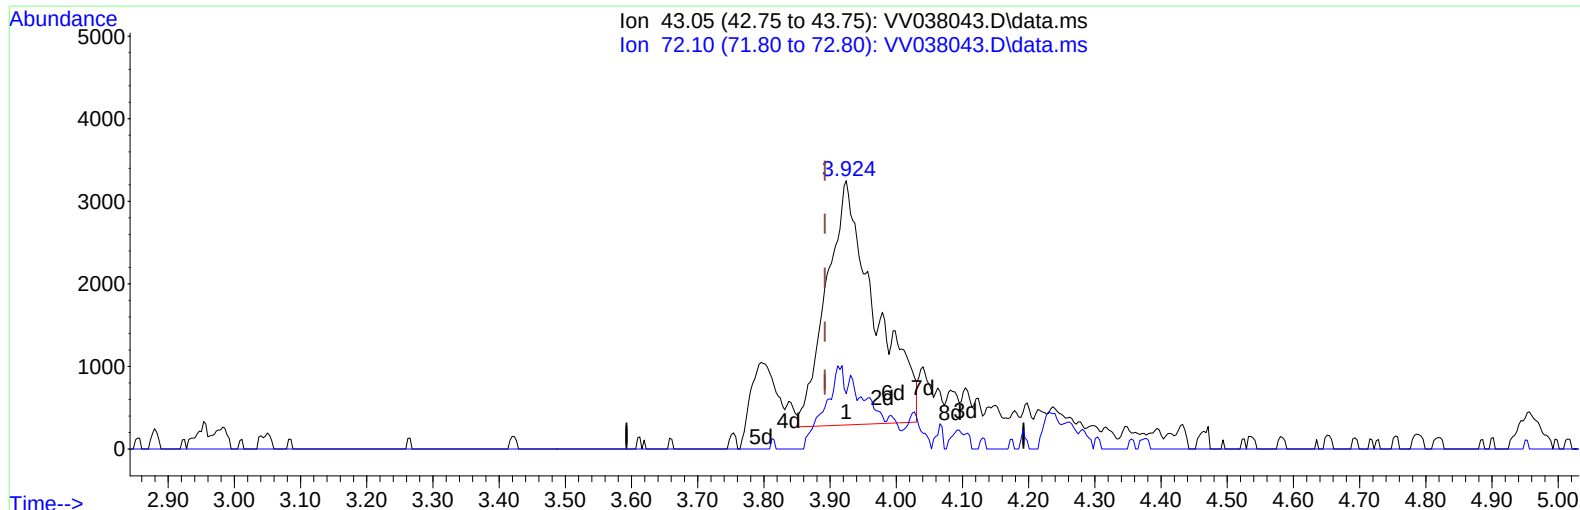

TIC: VV038043.D\data.ms

(21) 2-Butanone (T)

3.924min (+ 0.032) 4.21 ug/L m

response 15033

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	28.40	14.20#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
 Data File : VV038043.D
 Acq On : 13 Nov 2024 14:08
 Operator : SY/MD
 Sample : P4761-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AL6

Manual IntegrationsAPPROVED

Quant Time: Nov 13 23:11:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 13 00:39:48 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 11/14/2024
 Supervised By :Mahesh Dadoda 11/18/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	185651	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	196325	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	90052	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	69816	4.320	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	86.400%	
7) Chloroethane-d5	1.529	69	70567	5.357	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	107.200%	
11) 1,1-Dichloroethene-d2	2.056	65	33263	4.697	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	94.000%	
20) 2-Butanone-d5	3.789	46	209125	56.316	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	112.640%	
24) Chloroform-d	4.243	84	177253	5.819	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	116.400%	
26) 1,2-Dichloroethane-d4	4.937	65	83372	5.763	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	115.200%	
32) Benzene-d6	4.950	84	310117	5.113	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.200%	
36) 1,2-Dichloropropane-d6	5.982	67	100743	5.301	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.000%	
41) Toluene-d8	7.239	98	250347	4.513	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.200%	
43) trans-1,3-Dichloroprop...	7.558	79	33778	4.385	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.600%	
46) 2-Hexanone-d5	8.021	63	193104	56.076	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	112.160%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	86975	5.533	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	110.600%	
66) 1,2-Dichlorobenzene-d4	11.551	152	112153	5.990	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	119.800%	
Target Compounds					Qvalue	
13) Acetone	2.124	43	124176	46.912	ug/L	98
21) 2-Butanone	3.924	43	15033m	4.205	ug/L	
25) Chloroform	4.272	83	27631	0.954	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038043.D
Acq On : 13 Nov 2024 14:08
Operator : SY/MD
Sample : P4761-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AL6

Manual IntegrationsAPPROVED

Quant Time: Nov 13 23:11:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 13 00:39:48 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/14/2024
Supervised By :Mahesh Dadoda 11/18/2024

