

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
 Data File : VV038044.D
 Acq On : 13 Nov 2024 14:32
 Operator : SY/MD
 Sample : P4761-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0AL9

Quant Time: Nov 13 23:12:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 13 00:39:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	237191	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	248097	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	114344	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	69291	3.356	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.200%
7) Chloroethane-d5	1.529	69	66989	3.981	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.600%
11) 1,1-Dichloroethene-d2	2.053	65	31059	3.433	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.600%
20) 2-Butanone-d5	3.793	46	205064	43.223	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.440%
24) Chloroform-d	4.240	84	170760	4.388	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
26) 1,2-Dichloroethane-d4	4.937	65	83824	4.535	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.800%
32) Benzene-d6	4.953	84	302627	3.948	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.000%
36) 1,2-Dichloropropane-d6	5.982	67	99254	4.133	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.600%
41) Toluene-d8	7.239	98	238485	3.402	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.000%#
43) trans-1,3-Dichloroprop...	7.558	79	31681	3.254	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	65.000%
46) 2-Hexanone-d5	8.021	63	195681	44.967	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.940%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	84454	4.251	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.000%
66) 1,2-Dichlorobenzene-d4	11.554	152	109270	4.596	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.000%
Target Compounds					Qvalue	
13) Acetone	2.124	43	129130	38.183	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038044.D
Acq On : 13 Nov 2024 14:32
Operator : SY/MD
Sample : P4761-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0AL9

Quant Time: Nov 13 23:12:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 13 00:39:48 2024
Response via : Initial Calibration

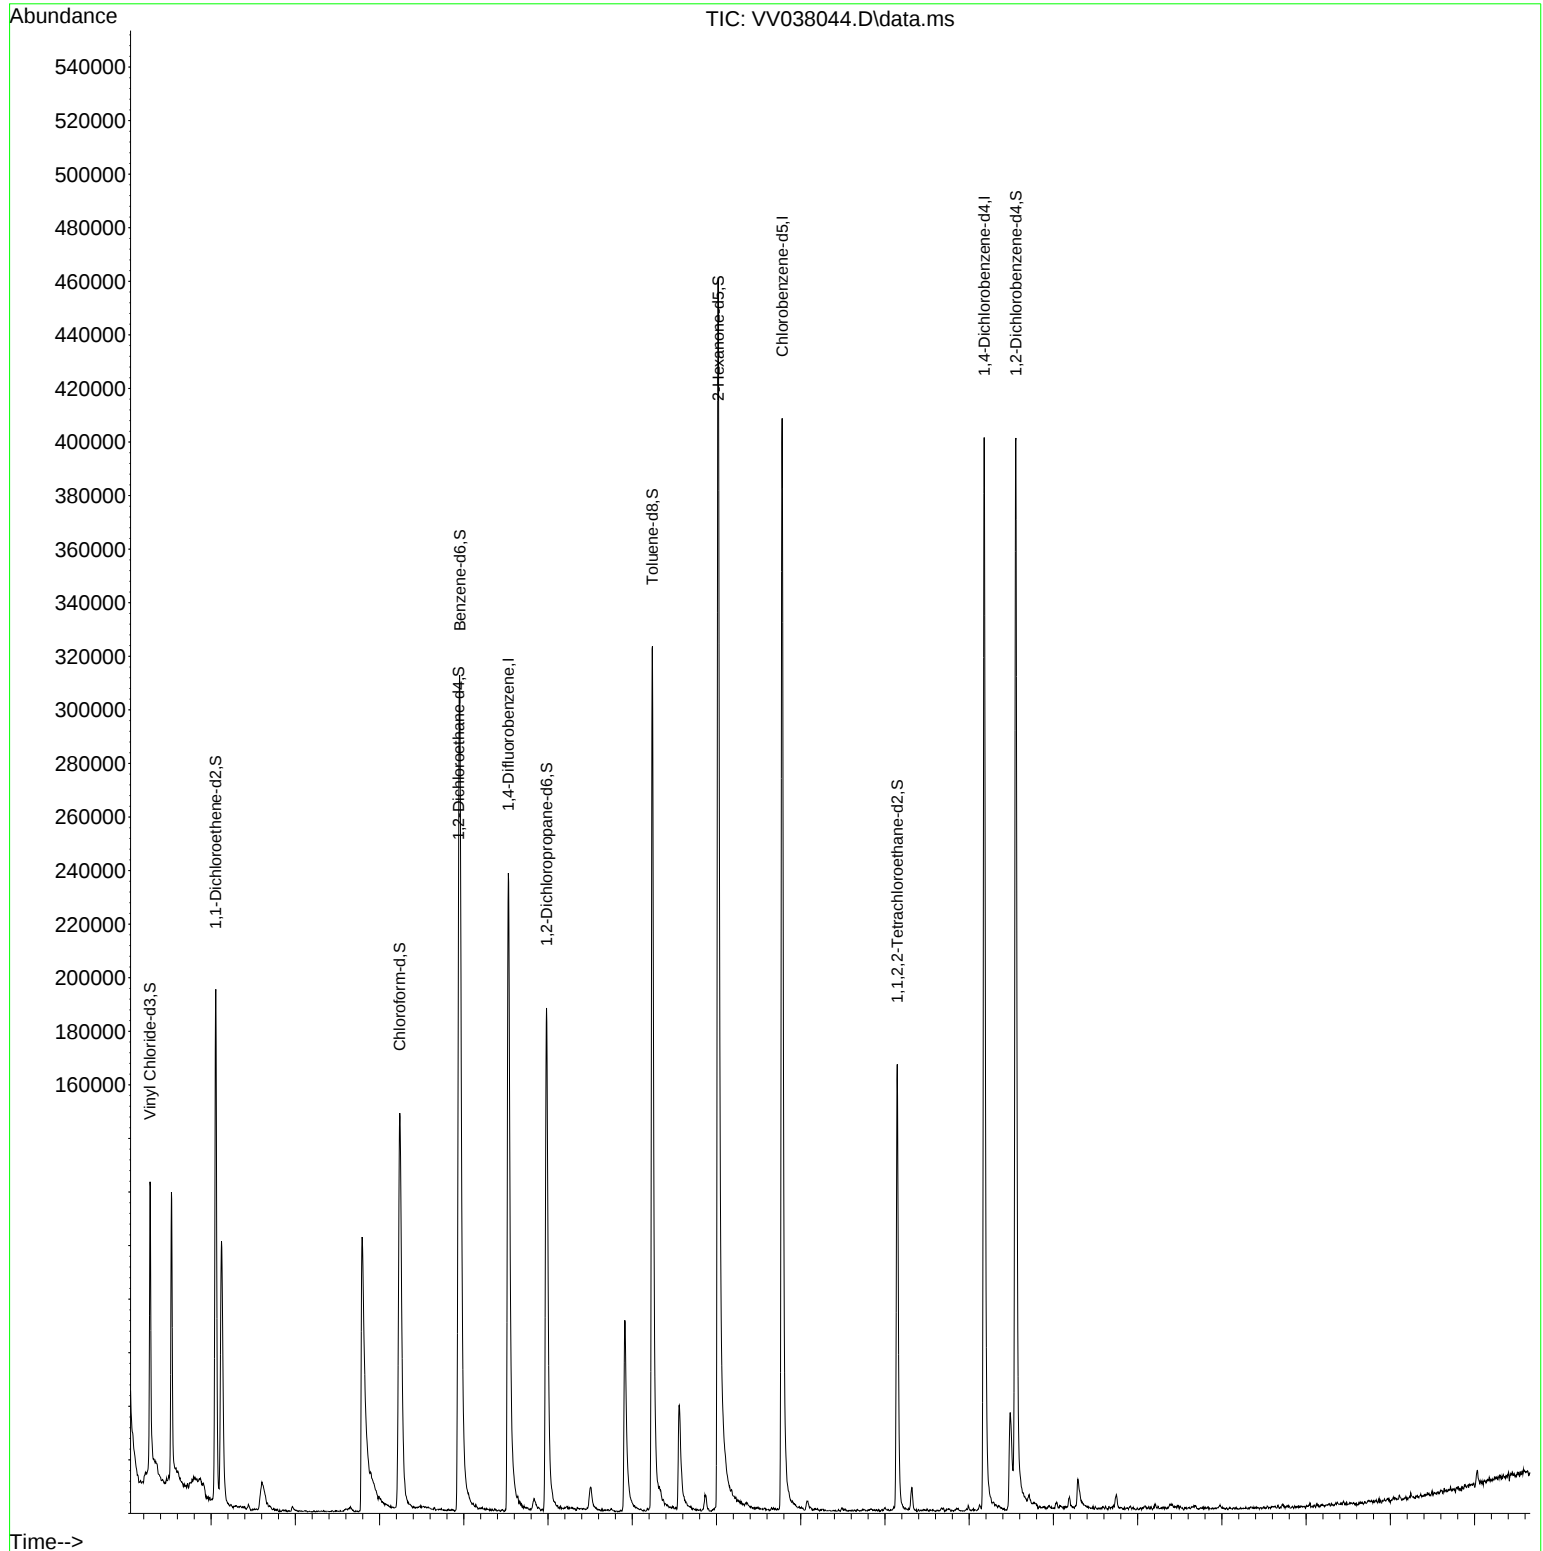

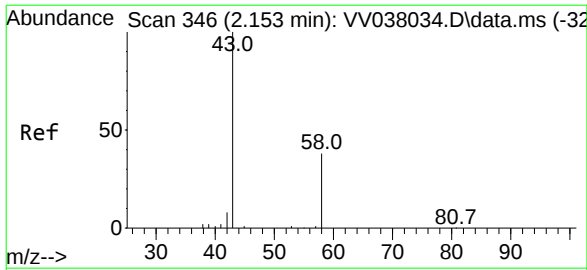

#13

Acetone

Concen: 38.183 ug/L

RT: 2.124 min Scan# 33

Delta R.T. -0.026 min

Lab File: VV038044.D

Acq: 13 Nov 2024 14:32

Instrument :

MSVOA_V

ClientSampleId :

A0AL9

Tgt Ion: 43 Resp: 129130

Ion Ratio Lower Upper

43 100

58 33.9 0.0 70.0

