

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
 Data File : VV038035.D
 Acq On : 13 Nov 2024 09:16
 Operator : SY/MD
 Sample : VV1113WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK254

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	93	rBV	161859	185984	17.20%	2.195%
2	1.529	145	152	162	rBV	142124	172220	15.93%	2.032%
3	2.053	303	315	334	rBV	262691	386434	35.75%	4.560%
4	3.834	855	869	897	rBV2	67355	326356	30.19%	3.851%
5	4.240	977	995	1022	rBV	180642	481914	44.58%	5.687%
6	4.950	1202	1216	1262	rBV2	404115	1081044	100.00%	12.757%
7	5.529	1386	1396	1424	rBV	257087	568101	52.55%	6.704%
8	5.982	1524	1537	1575	rBV	234817	523652	48.44%	6.179%
9	6.911	1816	1826	1860	rBV2	96225	210204	19.44%	2.480%
10	7.236	1914	1927	1959	rBV	423676	802605	74.24%	9.471%
11	7.555	2017	2026	2054	rBV2	56214	123904	11.46%	1.462%
12	8.024	2162	2172	2213	rBV	470254	1071315	99.10%	12.642%
13	8.358	2267	2276	2291	rBV2	25733	47947	4.44%	0.566%
14	8.780	2394	2407	2440	rBV	419099	752590	69.62%	8.881%
15	10.146	2821	2832	2854	rBV	195618	328242	30.36%	3.873%
16	11.178	3141	3153	3187	rBV	375805	644685	59.64%	7.607%
17	11.554	3258	3270	3294	rBV	433769	736010	68.08%	8.685%
18	14.821	4281	4286	4297	rBV	15027	14050	1.30%	0.166%
19	17.030	4965	4973	4979	rBV2	11517	17147	1.59%	0.202%




Sum of corrected areas: 8474404

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038035.D
Acq On : 13 Nov 2024 09:16
Operator : SY/MD
Sample : VV1113WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK254

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

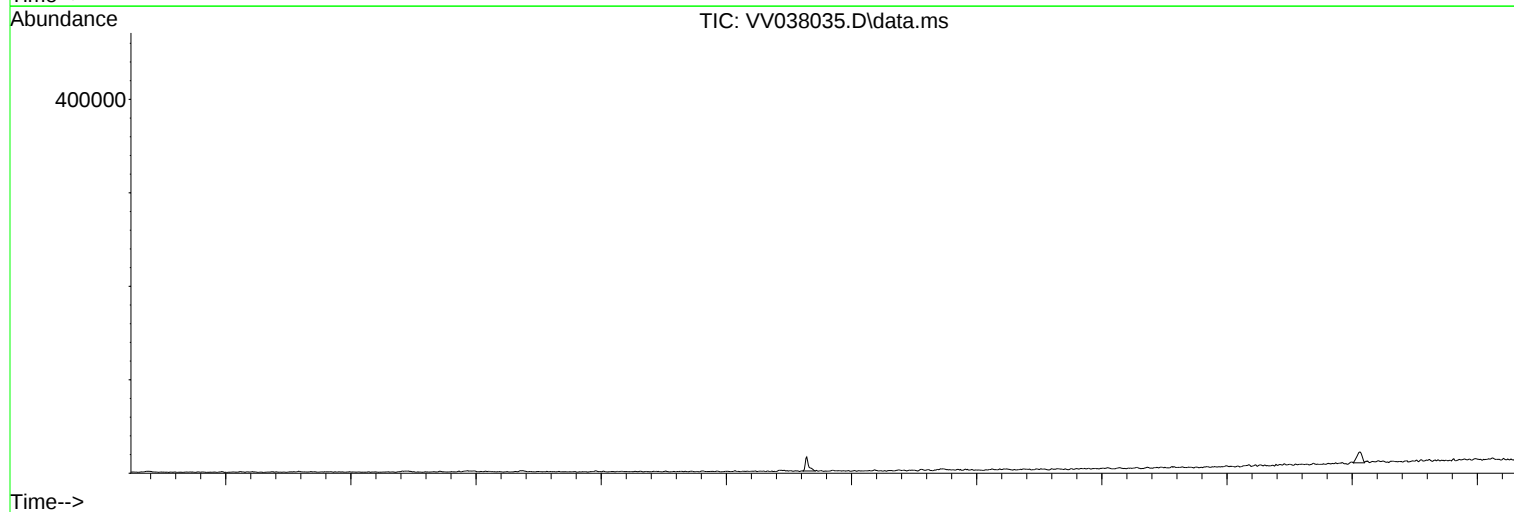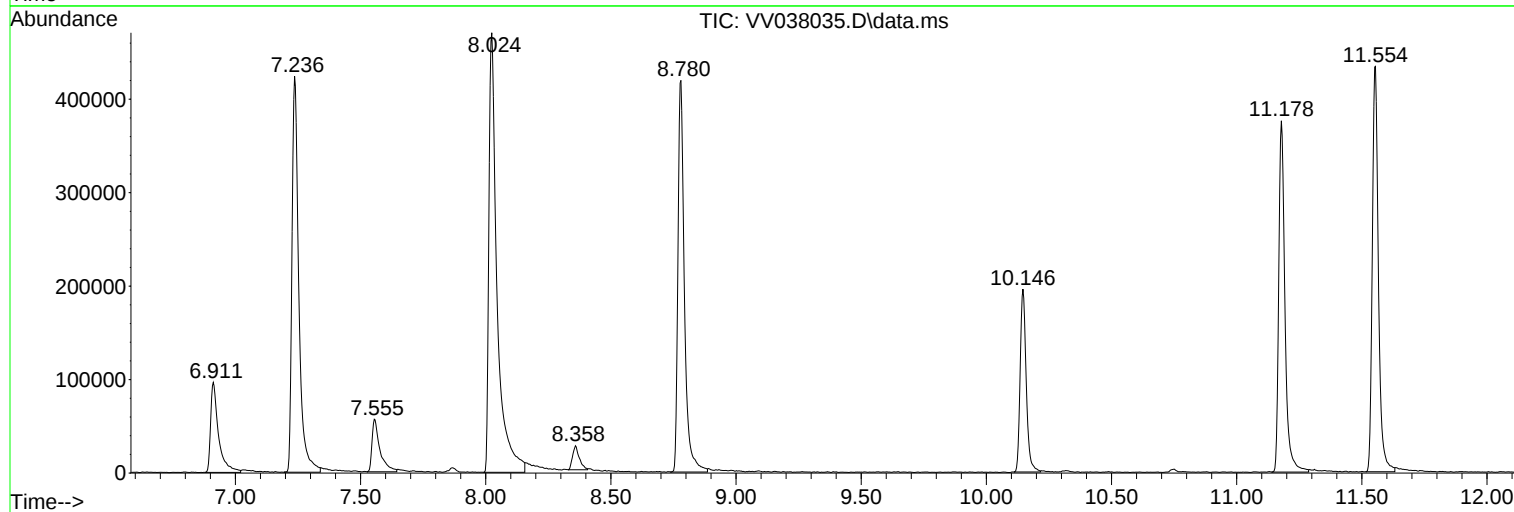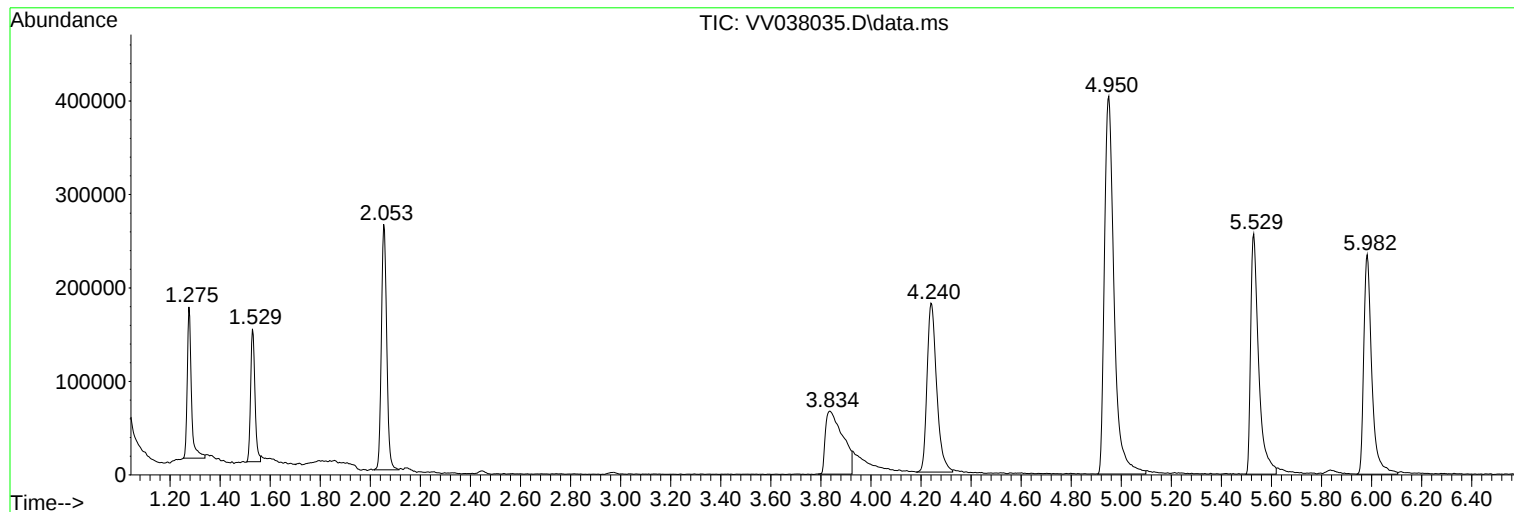

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038035.D
Acq On : 13 Nov 2024 09:16
Operator : SY/MD
Sample : VV1113WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK254

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038035.D
Acq On : 13 Nov 2024 09:16
Operator : SY/MD
Sample : VV1113WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK254

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------