

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
 Data File : VV038036.D
 Acq On : 13 Nov 2024 10:59
 Operator : SY/MD
 Sample : P4749-22DL 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GCP95DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV038036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	90	rBV2	926249	1013555	40.37%	4.432%
2	1.529	144	152	167	rBV	139782	172163	6.86%	0.753%
3	2.060	304	317	339	rBV4	690141	1146306	45.66%	5.012%
4	2.439	422	435	460	rBV	273252	465614	18.55%	2.036%
5	2.687	498	512	536	rBV	181639	328670	13.09%	1.437%
6	3.815	848	863	922	rBV4	108974	542454	21.61%	2.372%
7	4.236	978	994	1032	rVB3	175993	470116	18.73%	2.055%
8	4.497	1055	1075	1106	rBV	350222	908764	36.20%	3.973%
9	4.722	1127	1145	1165	rBV2	65774	161171	6.42%	0.705%
10	4.944	1199	1214	1228	rBV2	408760	1050002	41.82%	4.591%
11	5.526	1383	1395	1424	rBV	276620	611358	24.35%	2.673%
12	5.825	1473	1488	1518	rBV2	184765	409034	16.29%	1.788%
13	5.979	1523	1536	1557	rBV	231797	494726	19.71%	2.163%
14	6.082	1557	1568	1596	rVB	196464	415964	16.57%	1.819%
15	6.908	1815	1825	1845	rBV	100346	204432	8.14%	0.894%
16	7.233	1915	1926	1940	rBV	452643	821953	32.74%	3.594%
17	7.307	1940	1949	1977	rVB	470101	871885	34.73%	3.812%
18	7.551	2013	2025	2045	rBV2	59449	126882	5.05%	0.555%
19	7.760	2079	2090	2113	rBV	272426	491032	19.56%	2.147%
20	7.895	2118	2132	2160	rVB	604896	1047781	41.74%	4.581%
21	8.021	2160	2171	2212	rBV	454572	980426	39.05%	4.287%
22	8.355	2264	2275	2289	rBV3	33992	65014	2.59%	0.284%
23	8.776	2394	2406	2409	rBV	529139	719889	28.67%	3.148%
24	8.802	2410	2414	2447	rVV	798553	1344611	53.56%	5.879%
25	8.940	2447	2457	2483	rVV	136203	240520	9.58%	1.052%
26	9.063	2483	2495	2531	rVV	916661	1537658	61.25%	6.723%
27	9.471	2611	2622	2655	rBV3	246229	598275	23.83%	2.616%
28	10.095	2799	2816	2824	rBV3	146702	445958	17.76%	1.950%
29	10.143	2825	2831	2861	rVB2	230338	446118	17.77%	1.951%
30	11.197	3142	3159	3188	rBV2	1128747	2510534	100.00%	10.977%
31	11.558	3257	3271	3300	rBV2	670948	1629220	64.90%	7.123%
32	13.191	3767	3779	3810	rBV	351156	599513	23.88%	2.621%




Sum of corrected areas: 22871598

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038036.D
Acq On : 13 Nov 2024 10:59
Operator : SY/MD
Sample : P4749-22DL 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GCP95DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

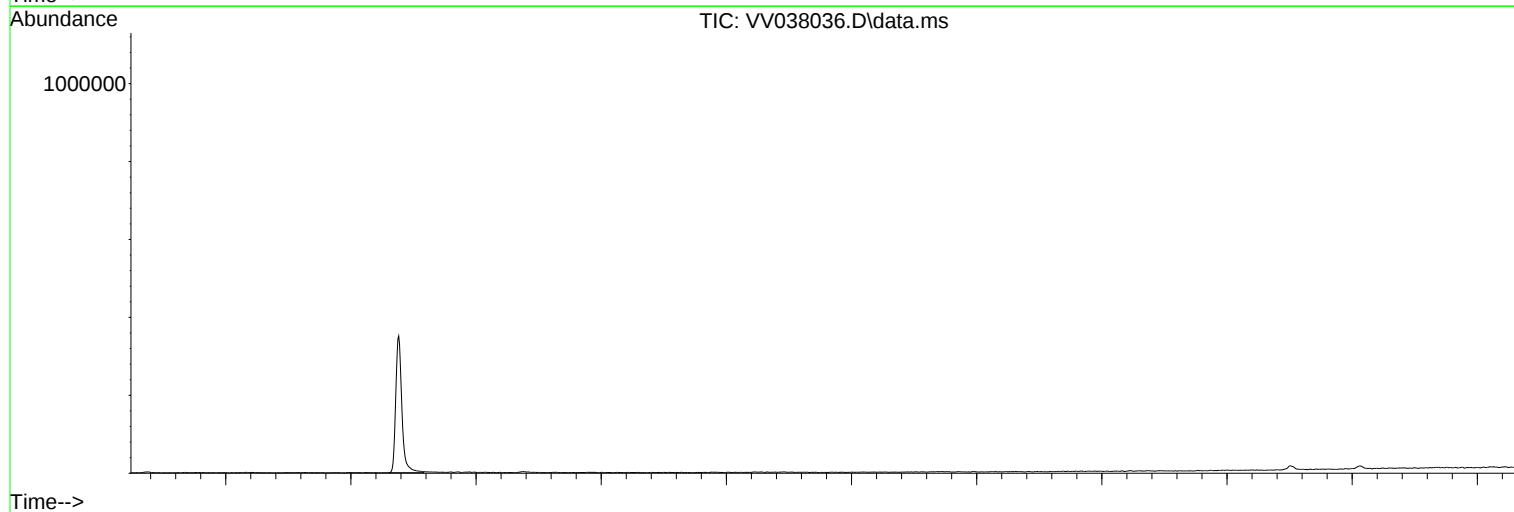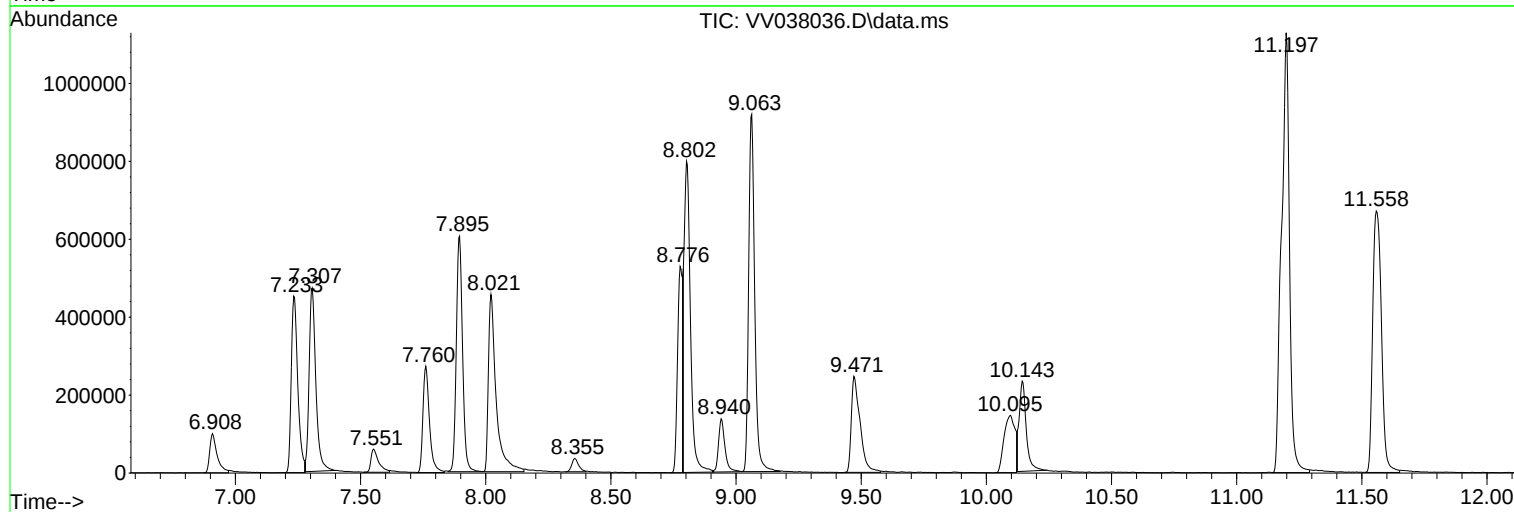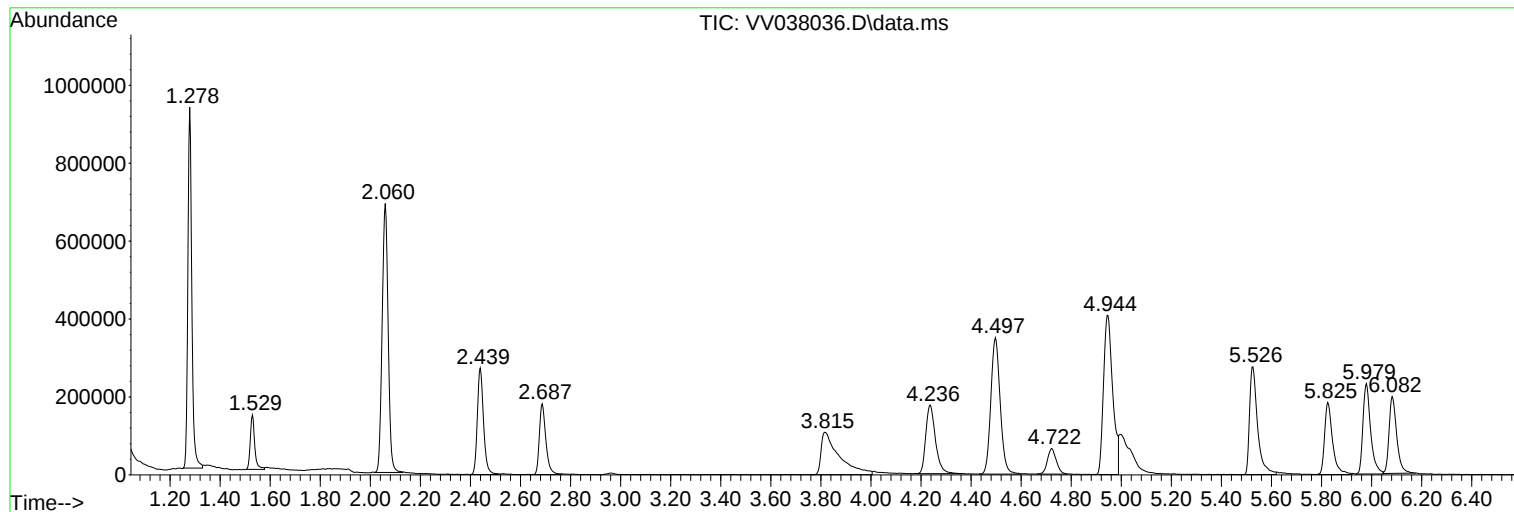

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038036.D
Acq On : 13 Nov 2024 10:59
Operator : SY/MD
Sample : P4749-22DL 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GCP95DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1,3,5-trichloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD		R.T.	
10.095	0.89 ug/L	445958	1,4-Dichlorobenzene-d4		11.175	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Benzene, 1,3,5-trichloro-		180	C6H3Cl3	000108-70-3	98
2	Benzene, 1,2,3-trichloro-		180	C6H3Cl3	000087-61-6	98
3	Benzene, 1,2,3-trichloro-		180	C6H3Cl3	000087-61-6	98
4	Benzene, 1,2,4-trichloro-		180	C6H3Cl3	000120-82-1	98
5	Benzene, 1,3,5-trichloro-		180	C6H3Cl3	000108-70-3	98

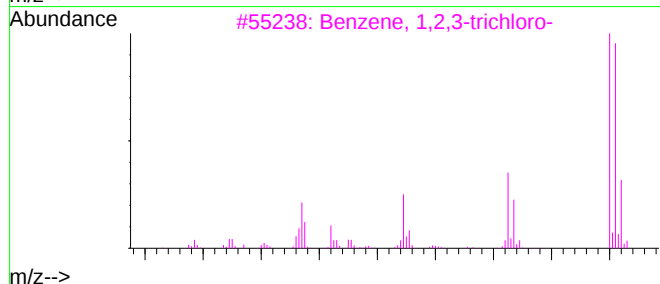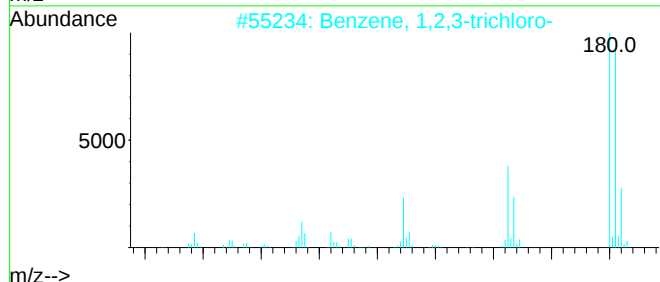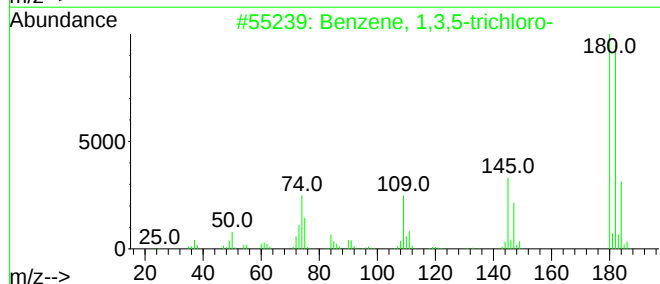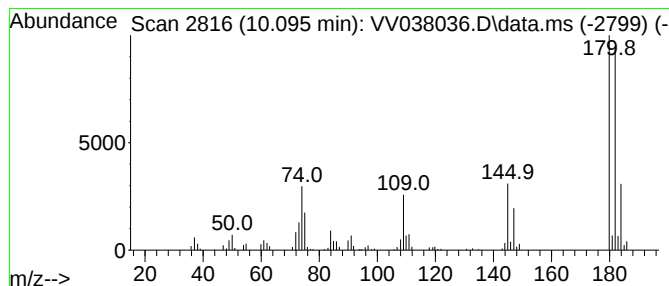

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038036.D
Acq On : 13 Nov 2024 10:59
Operator : SY/MD
Sample : P4749-22DL 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GCP95DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3,5-...	10.095	0.9	ug/L	445958	3	11.175	2510530	5.0