

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
 Data File : VV038042.D
 Acq On : 13 Nov 2024 13:44
 Operator : SY/MD
 Sample : P4761-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A0ALO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	88	rVB	98654	108357	12.15%	1.637%
2	1.352	93	97	113	rVB	13456	24051	2.70%	0.363%
3	1.529	145	152	162	rBV	96753	116848	13.10%	1.765%
4	2.053	306	315	328	rBV	176747	258139	28.94%	3.899%
5	2.307	376	394	396	rBV6	8910	17465	1.96%	0.264%
6	3.802	842	859	905	rBV2	126052	479417	53.75%	7.241%
7	4.243	981	996	1026	rBV2	142985	421317	47.24%	6.364%
8	4.950	1202	1216	1246	rBV2	287350	757152	84.89%	11.436%
9	5.529	1387	1396	1429	rBV	178042	404790	45.39%	6.114%
10	5.982	1524	1537	1570	rBV	172508	386192	43.30%	5.833%
11	6.912	1815	1826	1860	rBV2	65068	151013	16.93%	2.281%
12	7.236	1917	1927	1952	rBV	296975	564925	63.34%	8.533%
13	7.558	2016	2027	2050	rBV2	36793	85230	9.56%	1.287%
14	8.021	2162	2171	2217	rBV	414255	891902	100.00%	13.472%
15	8.780	2396	2407	2446	rBV	302999	549423	61.60%	8.299%
16	10.146	2822	2832	2857	rBV	145945	245068	27.48%	3.702%
17	10.317	2875	2885	2897	rVB5	8623	14918	1.67%	0.225%
18	11.178	3143	3153	3174	rBV	292036	489557	54.89%	7.394%
19	11.506	3242	3255	3259	rBV3	11069	19865	2.23%	0.300%
20	11.555	3259	3270	3295	rVB	356053	602813	67.59%	9.105%
21	12.288	3487	3498	3518	rBV6	14846	32129	3.60%	0.485%




Sum of corrected areas: 6620571

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038042.D
Acq On : 13 Nov 2024 13:44
Operator : SY/MD
Sample : P4761-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0ALO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

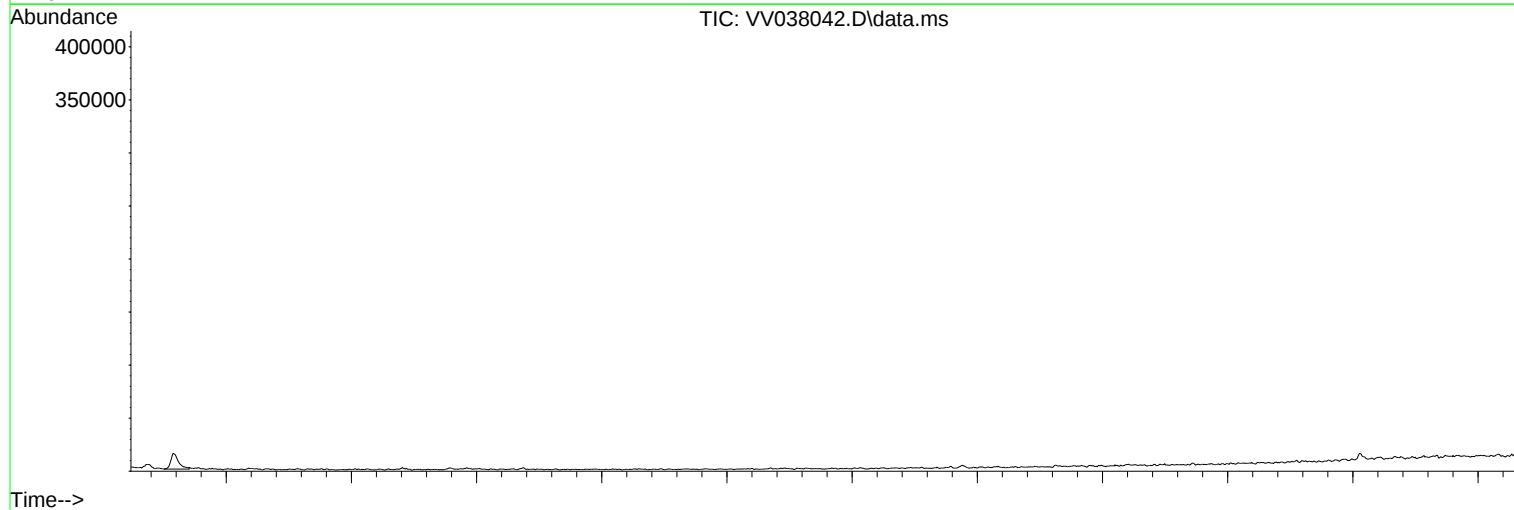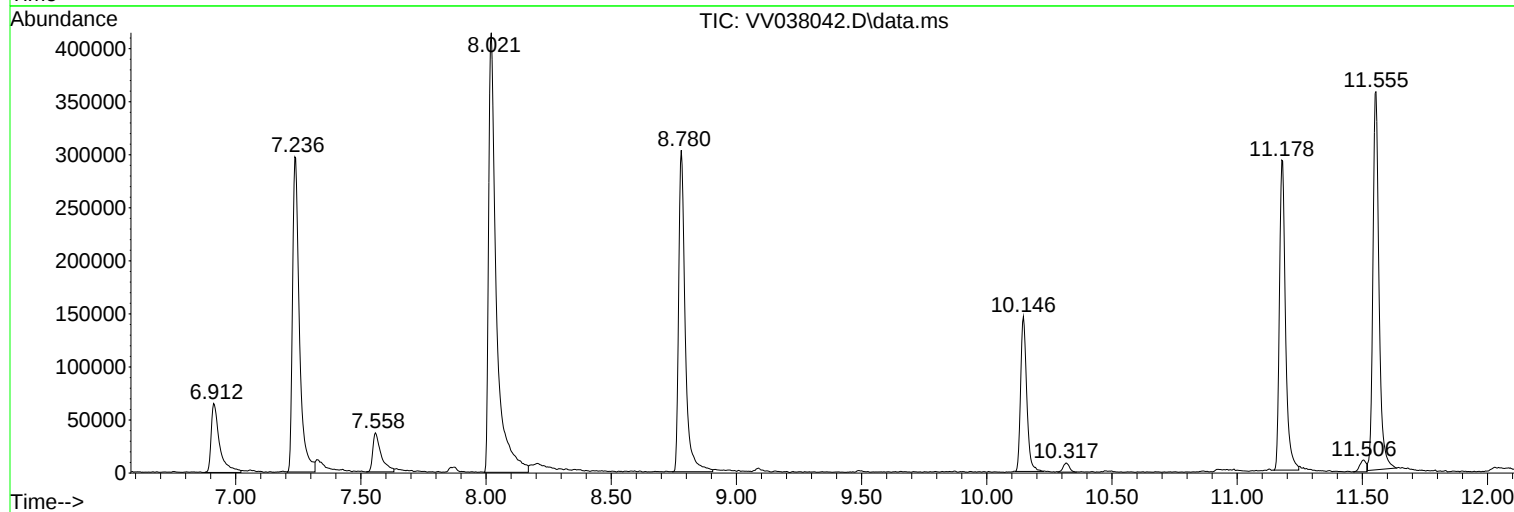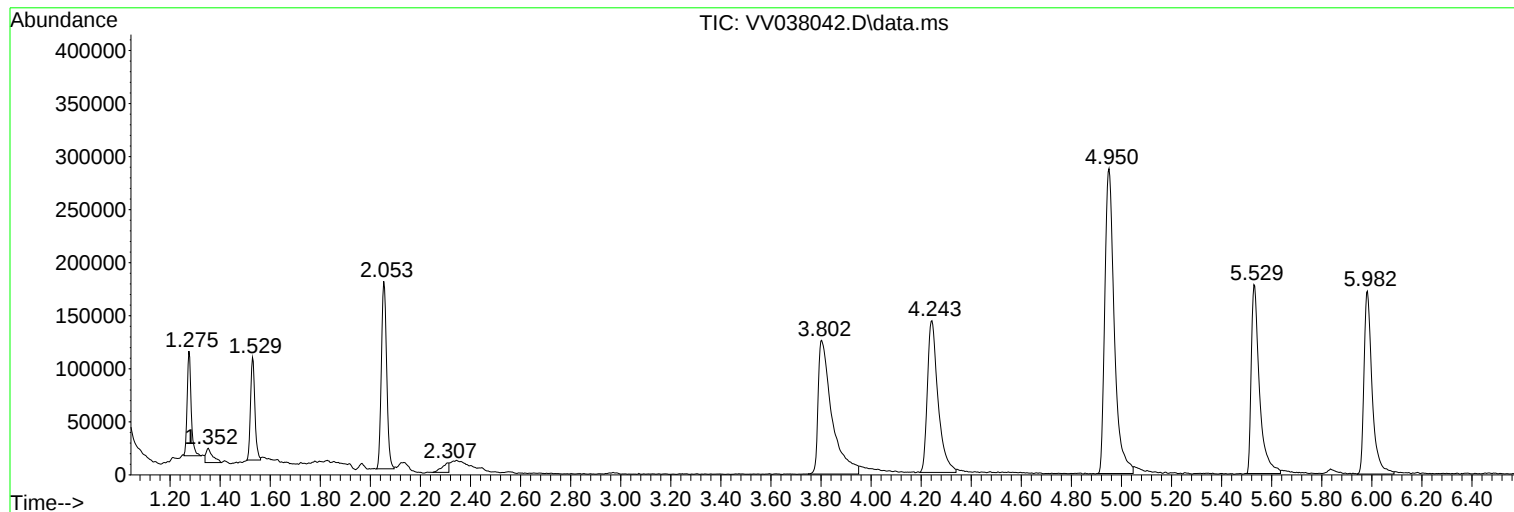

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038042.D
Acq On : 13 Nov 2024 13:44
Operator : SY/MD
Sample : P4761-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0ALO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038042.D
Acq On : 13 Nov 2024 13:44
Operator : SY/MD
Sample : P4761-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A0ALO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------