

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
 Data File : VV038060.D
 Acq On : 13 Nov 2024 21:35
 Operator : SY/MD
 Sample : P4804-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46Q9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	65	73	81	rBV	64581	77778	12.64%	1.990%
2	1.346	90	95	109	rVB	23134	30888	5.02%	0.790%
3	1.529	145	152	166	rBV	56226	71580	11.63%	1.832%
4	2.053	304	315	326	rBV	99994	150894	24.52%	3.861%
5	2.108	326	332	343	rVB2	11038	17705	2.88%	0.453%
6	3.783	843	853	890	rBV	74626	236574	38.44%	6.054%
7	4.243	980	996	1020	rBV2	74287	202432	32.89%	5.180%
8	4.950	1203	1216	1252	rBV4	164049	447230	72.67%	11.445%
9	5.532	1383	1397	1435	rBV2	103530	253682	41.22%	6.492%
10	5.985	1526	1538	1560	rBV	96535	214330	34.83%	5.485%
11	6.918	1817	1828	1858	rBV3	32903	80328	13.05%	2.056%
12	7.239	1918	1928	1951	rBV	142652	282956	45.98%	7.241%
13	7.564	2020	2029	2049	rBV3	20081	46592	7.57%	1.192%
14	7.870	2112	2124	2138	rVB3	8313	15783	2.56%	0.404%
15	8.017	2161	2170	2207	rBV	284975	615439	100.00%	15.750%
16	8.779	2398	2407	2441	rBV	180994	357801	58.14%	9.156%
17	10.146	2821	2832	2853	rBV	108943	184018	29.90%	4.709%
18	10.320	2876	2886	2899	rVB3	9639	15334	2.49%	0.392%
19	11.181	3144	3154	3180	rBV	166361	291457	47.36%	7.459%
20	11.554	3255	3270	3289	rBV	179965	308556	50.14%	7.896%
21	17.027	4968	4972	4982	rVB8	3988	6308	1.02%	0.161%

Sum of corrected areas: 3907665




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038060.D
Acq On : 13 Nov 2024 21:35
Operator : SY/MD
Sample : P4804-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46Q9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

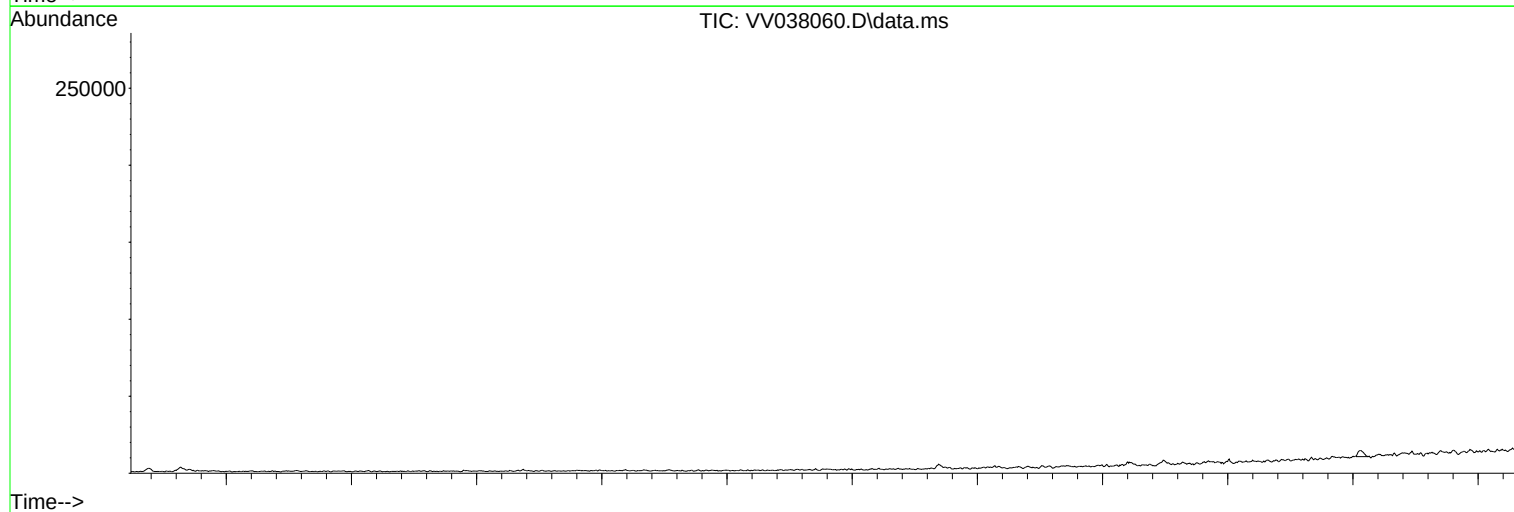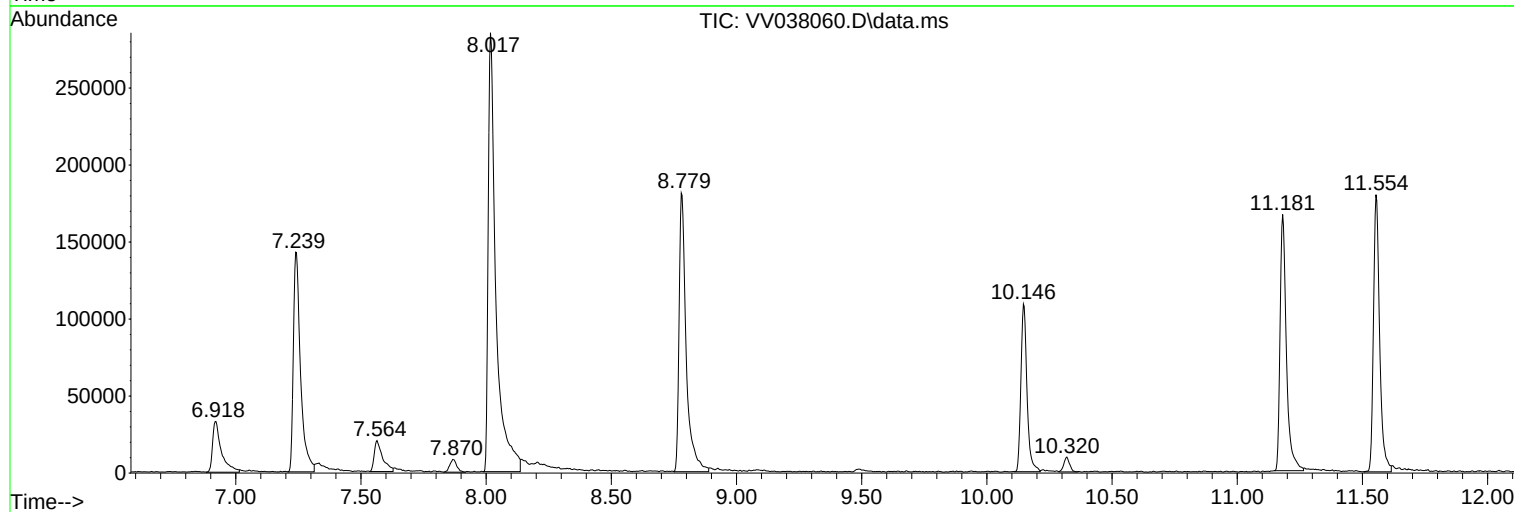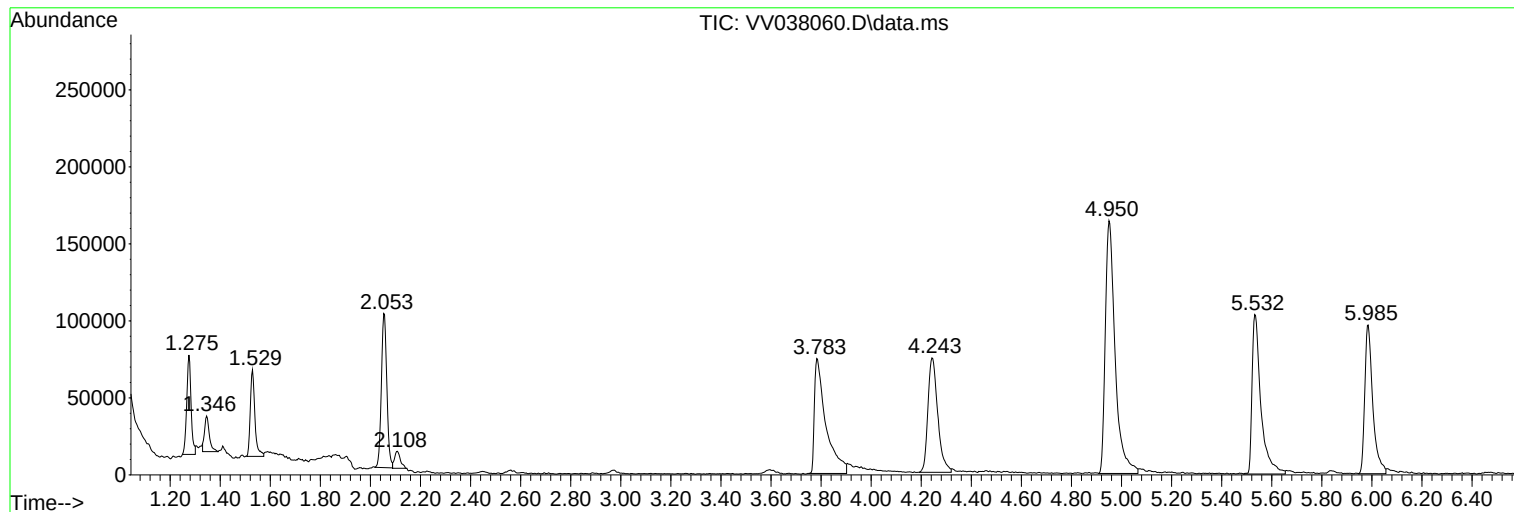

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038060.D
Acq On : 13 Nov 2024 21:35
Operator : SY/MD
Sample : P4804-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46Q9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111324\
Data File : VV038060.D
Acq On : 13 Nov 2024 21:35
Operator : SY/MD
Sample : P4804-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46Q9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
