

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038094.D
 Acq On : 14 Nov 2024 18:56
 Operator : SY/MD
 Sample : P4803-02
 Misc : 26mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 00:33:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9297	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	9083	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	4511	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	5846	0.607	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 122.000%			
4) 1,2-Dichloroethane-d4	4.969	65	3460	0.593	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 118.000%			
7) 1,2-Dichloropropane-d6	5.995	67	4130	0.561	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 112.000%			
8) Toluene-d8	7.253	98	10390	0.551	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 110.000%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3287	0.559	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 112.000%			
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.305	75	17	0.022	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038094.D
Acq On : 14 Nov 2024 18:56
Operator : SY/MD
Sample : P4803-02
Misc : 26mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 15 00:33:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

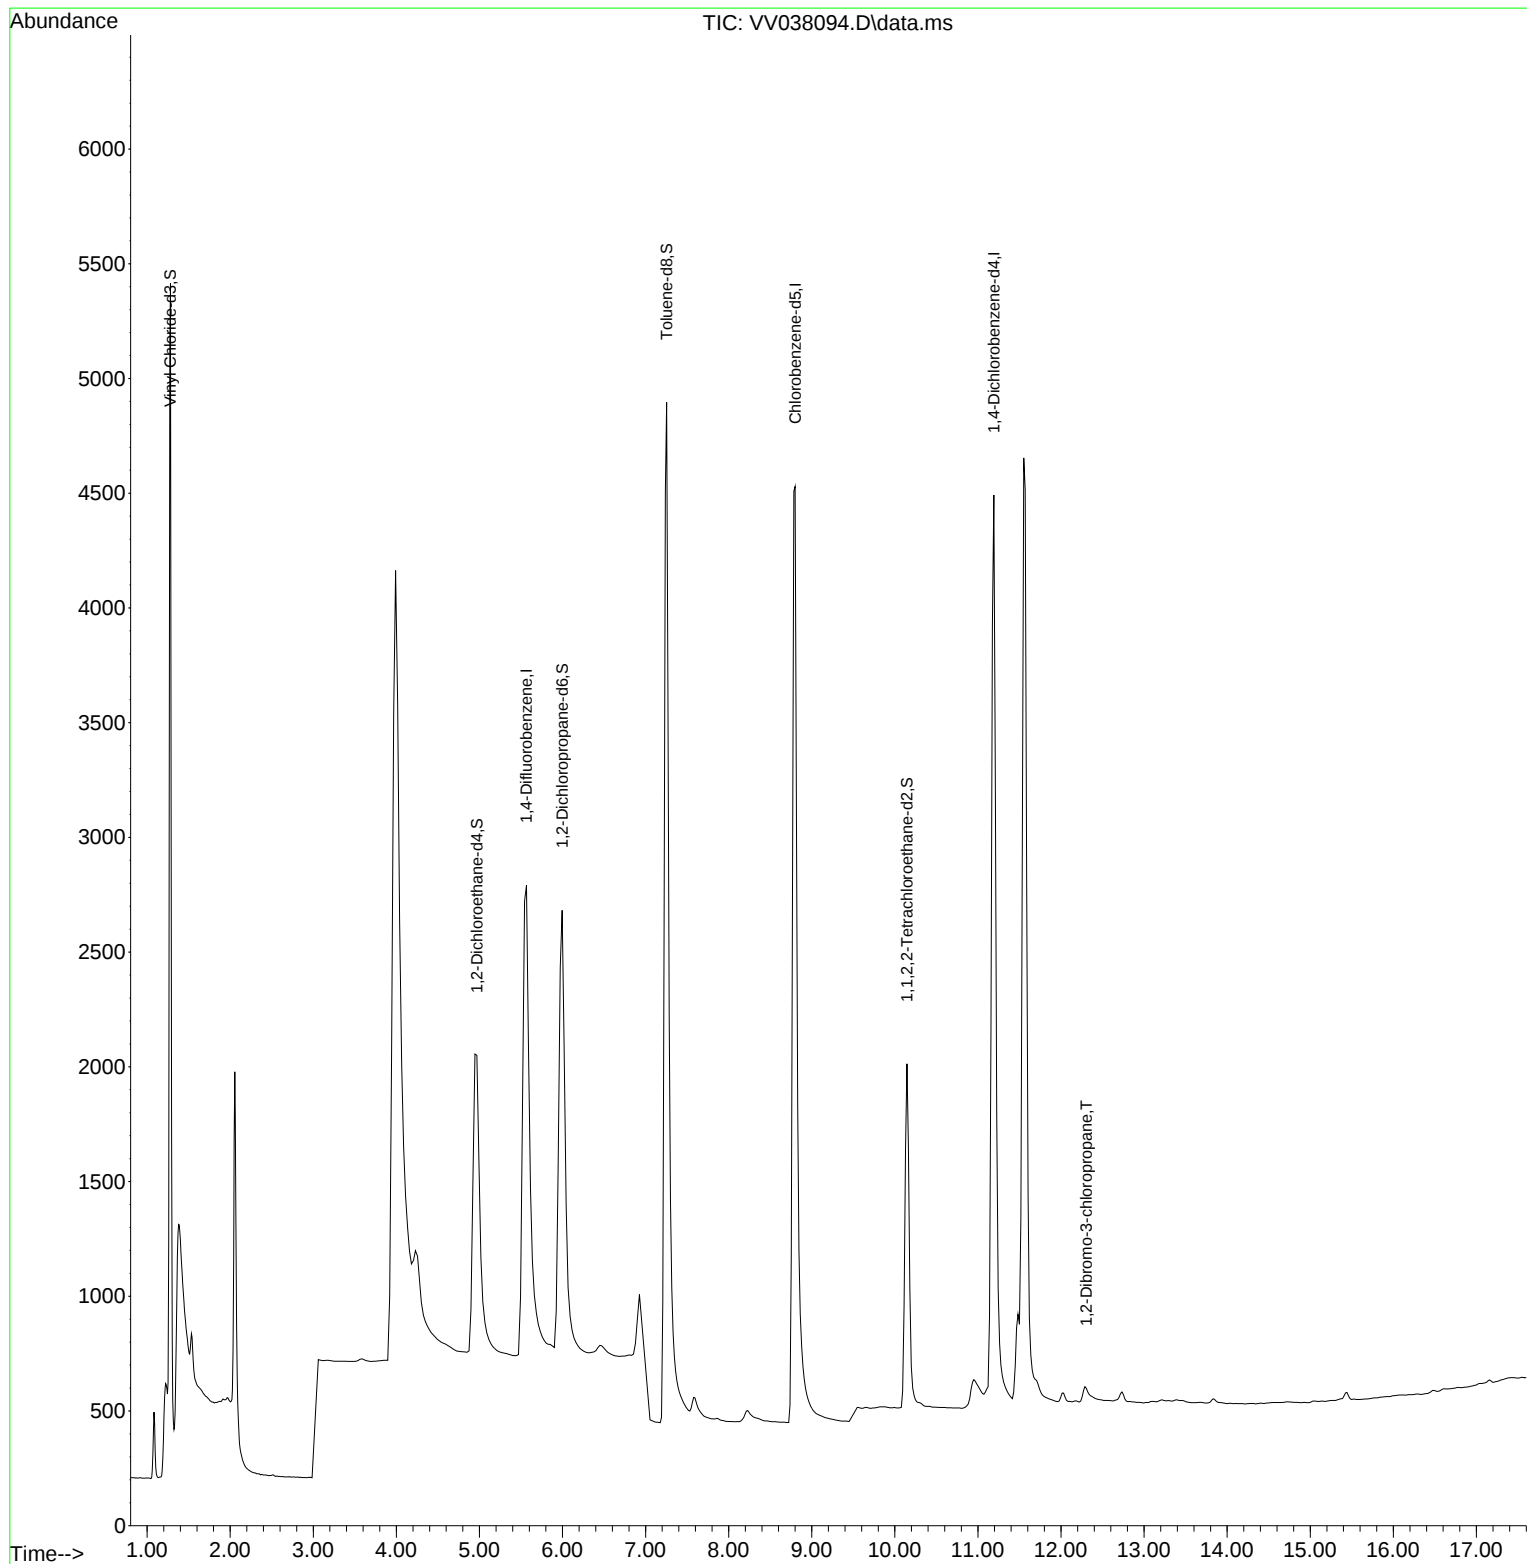

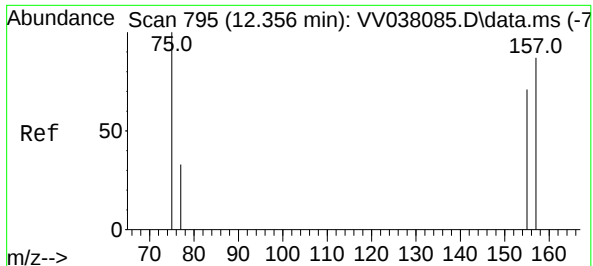

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.022 ug/L
 RT: 12.305 min Scan# 79
 Delta R.T. -0.051 min
 Lab File: VV038094.D
 Acq: 14 Nov 2024 18:56

Instrument :
 MSVOA_V
 ClientSampleId :

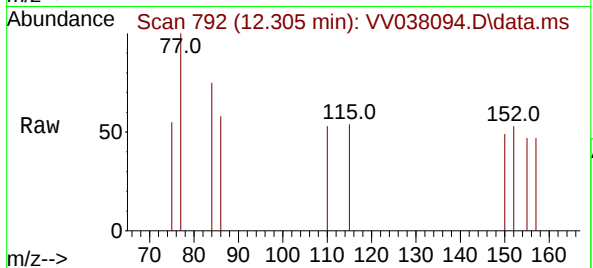

Tgt Ion: 75 Resp: 17
 Ion Ratio Lower Upper
 75 100
 157 85.7 69.4 104.0
 155 85.7 61.3 91.9

