

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038099.D
 Acq On : 14 Nov 2024 20:56
 Operator : SY/MD
 Sample : P4761-02 2X
 Misc : 26mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 00:34:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9802	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	9826	0.500	ug/L	#-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	5118	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	5663	0.557	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	112.000%
4) 1,2-Dichloroethane-d4	4.969	65	3482	0.566	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	114.000%
7) 1,2-Dichloropropane-d6	5.995	67	4674	0.587	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	118.000%
8) Toluene-d8	7.253	98	11002	0.540	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3239	0.509	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	102.000%
Target Compounds						
3) Vinyl chloride	1.379	62	512	0.051	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038099.D
Acq On : 14 Nov 2024 20:56
Operator : SY/MD
Sample : P4761-02 2X
Misc : 26mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 15 00:34:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration

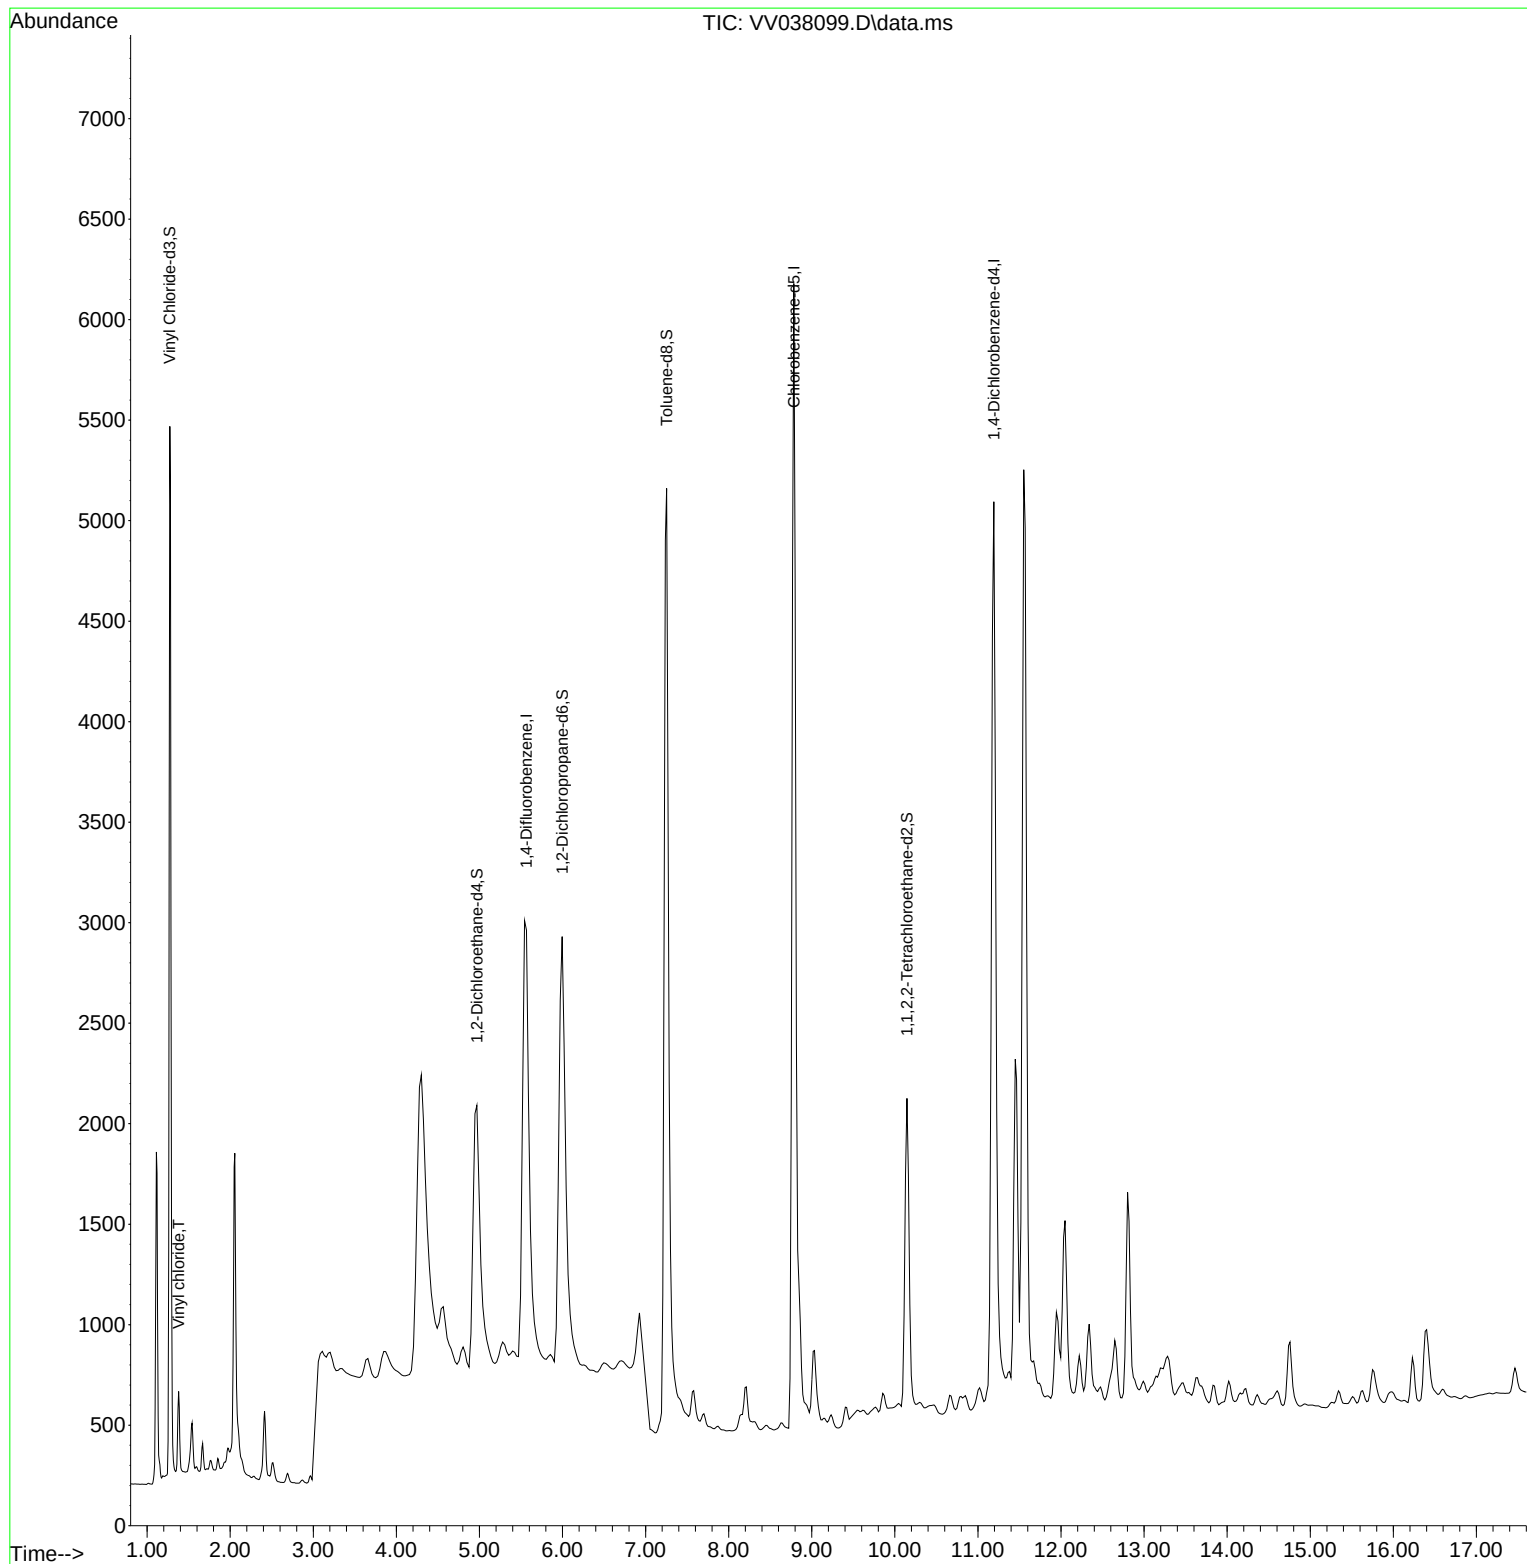

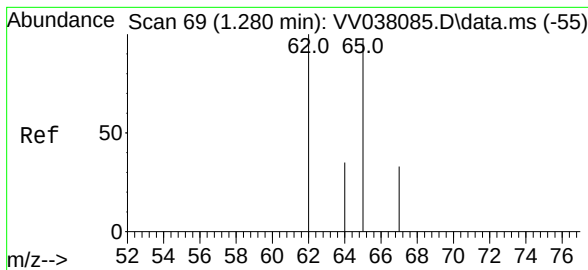

#3

Vinyl chloride

Concen: 0.051 ug/L

RT: 1.379 min Scan# 84

Delta R.T. 0.099 min


Lab File: VV038099.D

Acq: 14 Nov 2024 20:56

Instrument :

MSVOA_V

ClientSampleId :

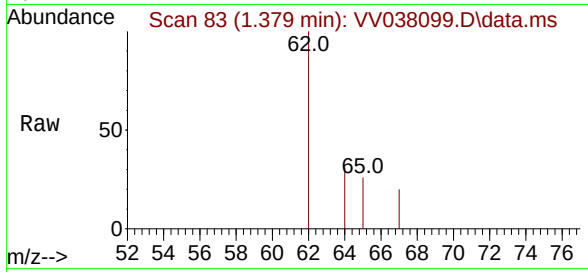

Tgt Ion: 62 Resp: 512

Ion Ratio Lower Upper

62 100

64 31.2 25.3 47.1

