

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
 Data File : VV038101.D
 Acq On : 14 Nov 2024 21:44
 Operator : SY/MD
 Sample : P4761-05 2X
 Misc : 26mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 15 00:35:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 00:15:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	10083	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	10317	0.500	ug/L	#-0.02
11) 1,4-Dichlorobenzene-d4	11.191	152	5044	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.287	65	5623	0.538	ug/L	0.01
Spiked Amount	0.500	Range	40 - 130	Recovery	=	108.000%
4) 1,2-Dichloroethane-d4	4.969	65	3522	0.557	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	112.000%
7) 1,2-Dichloropropane-d6	6.019	67	4885	0.585	ug/L	0.02
Spiked Amount	0.500	Range	60 - 140	Recovery	=	116.000%
8) Toluene-d8	7.253	98	11204	0.524	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3110	0.466	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	94.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.386	62	815	0.078	ug/L	83
12) 1,2,3-Trichloropropane	9.991	75	94	0.021	ug/L #	1
13) 1,2-Dibromo-3-chloropr...	12.322	75	54	0.062	ug/L #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111424\
Data File : VV038101.D
Acq On : 14 Nov 2024 21:44
Operator : SY/MD
Sample : P4761-05 2X
Misc : 26mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 15 00:35:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 00:15:53 2024
Response via : Initial Calibration




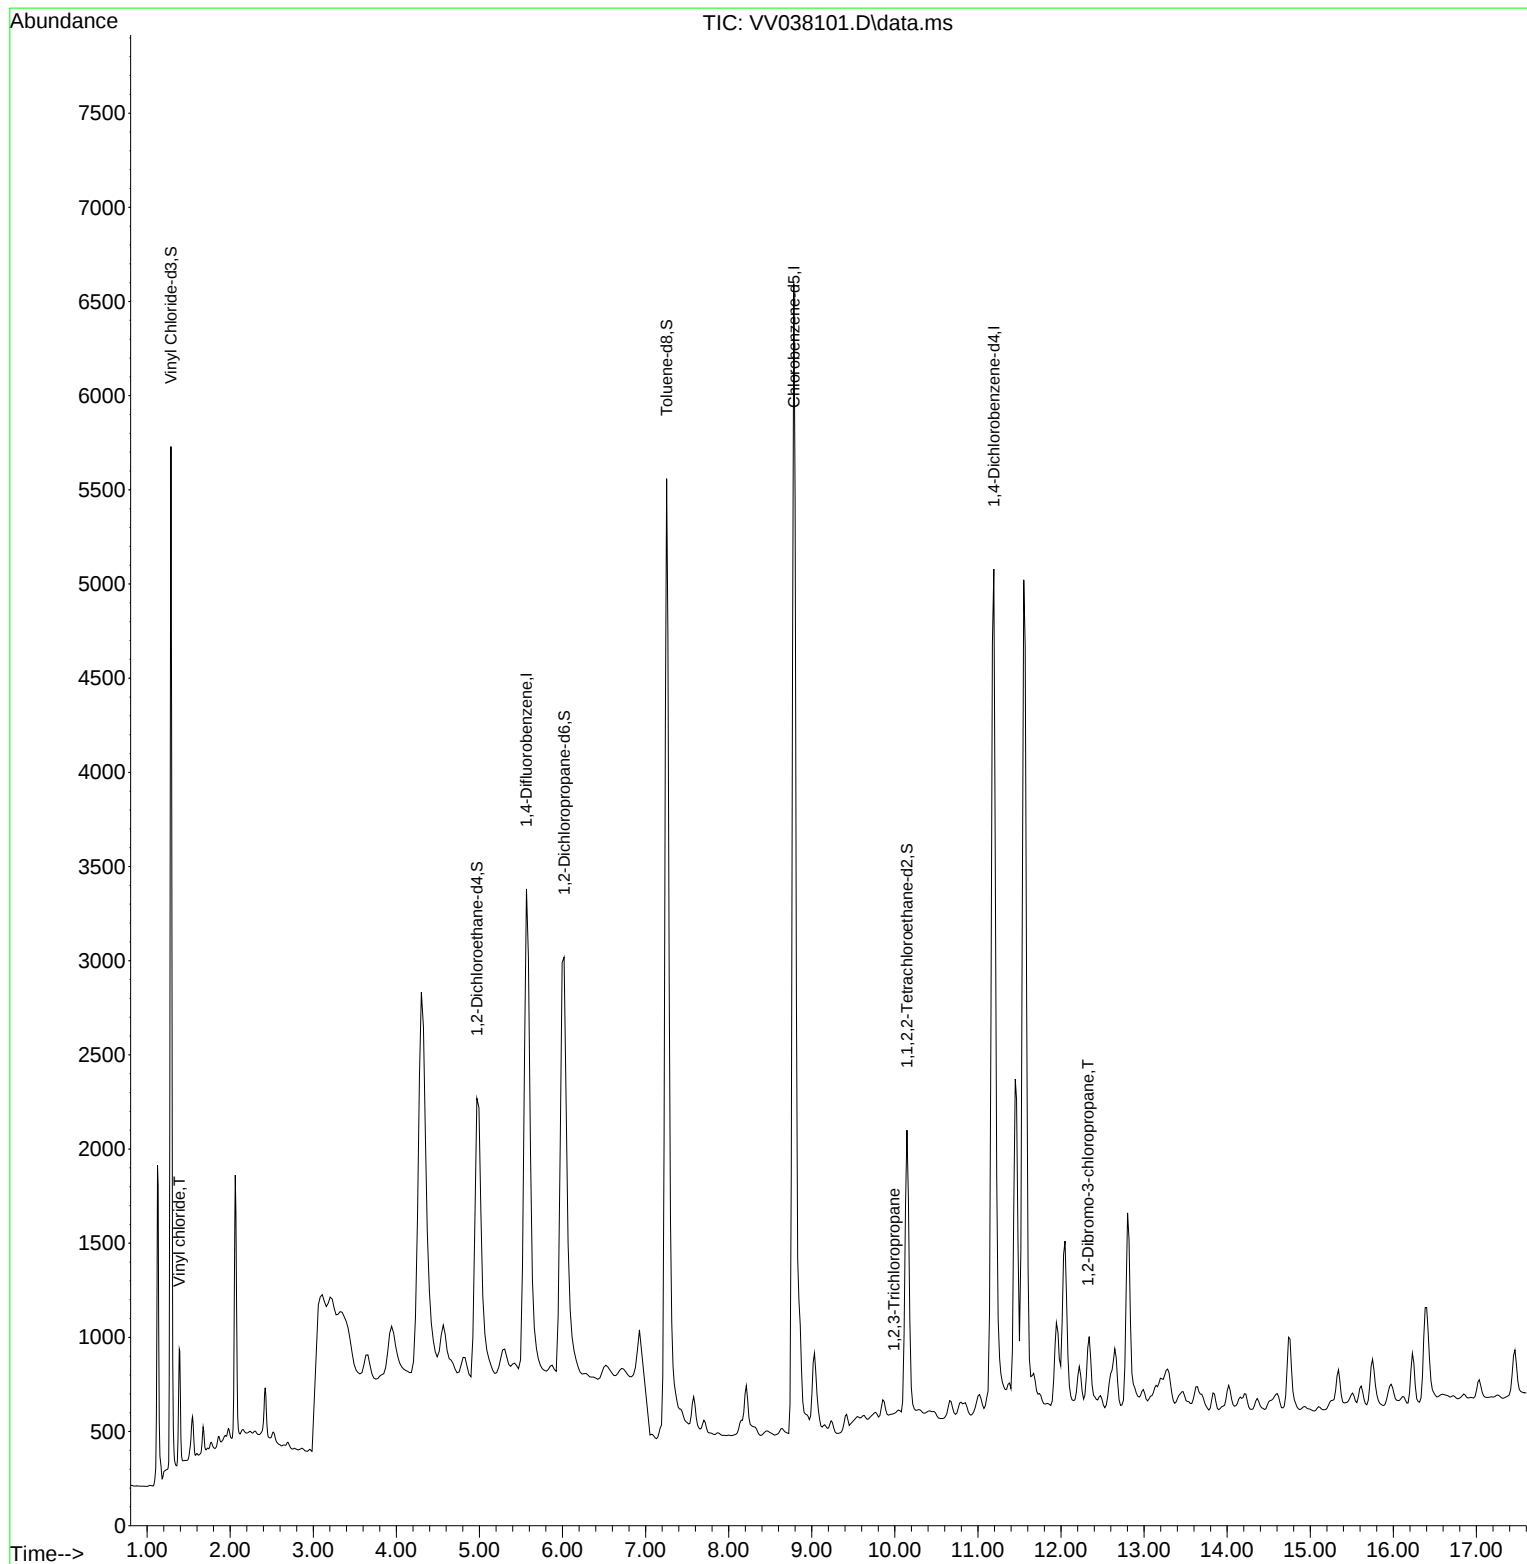


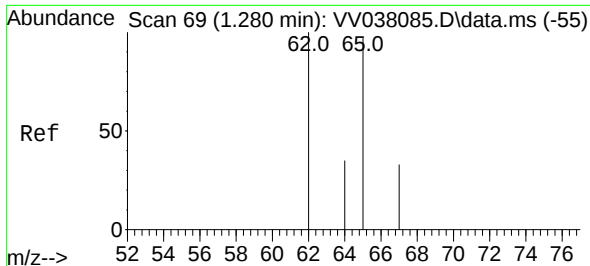

#3
 Vinyl chloride
 Concen: 0.078 ug/L
 RT: 1.386 min Scan# 84
 Delta R.T. 0.106 min
 Lab File: VV038101.D
 Acq: 14 Nov 2024 21:44




Instrument :
 MSVOA_V
 ClientSampleId :


Tgt Ion: 62 Resp: 815
 Ion Ratio Lower Upper
 62 100
 64 26.4 25.3 47.1

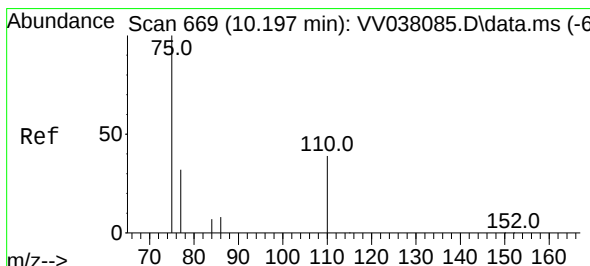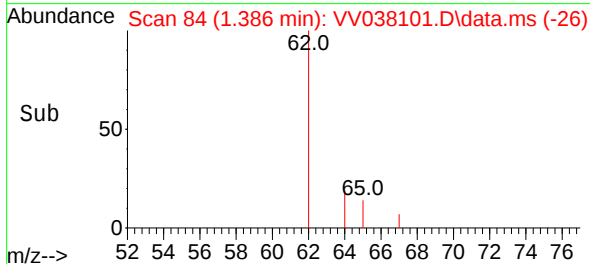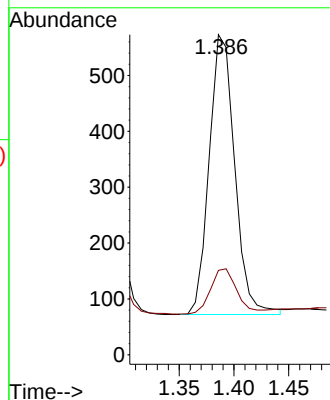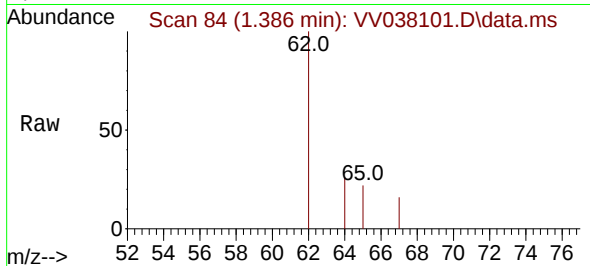

#12
 1,2,3-Trichloropropane
 Concen: 0.021 ug/L
 RT: 9.991 min Scan# 657
 Delta R.T. -0.206 min
 Lab File: VV038101.D
 Acq: 14 Nov 2024 21:44


Tgt Ion: 75 Resp: 94
 Ion Ratio Lower Upper
 75 100
 110 16.0 34.3 51.5#
 77 167.0 26.6 40.0#

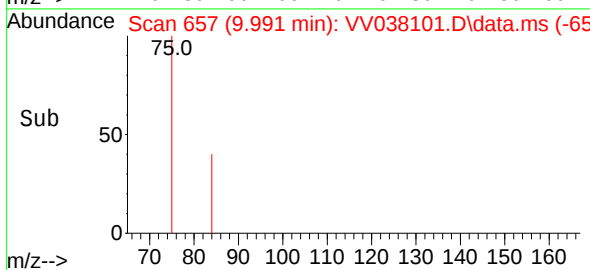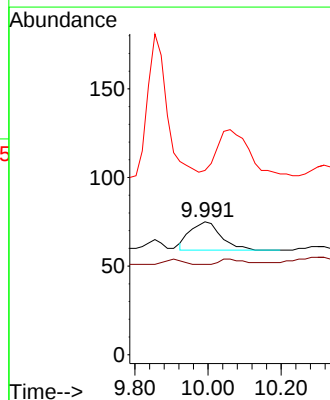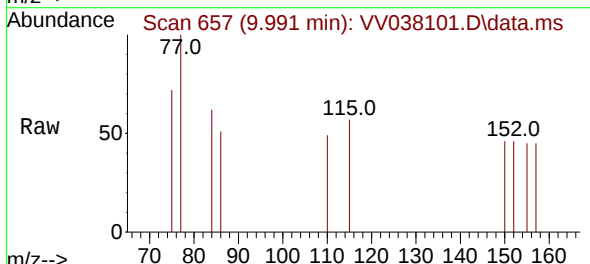

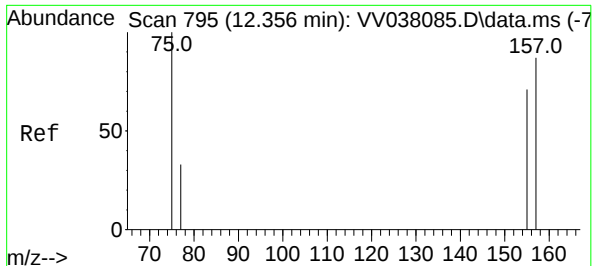

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.062 ug/L
 RT: 12.322 min Scan# 79
 Delta R.T. -0.034 min
 Lab File: VV038101.D
 Acq: 14 Nov 2024 21:44

Instrument :
 MSVOA_V
 ClientSampleId :

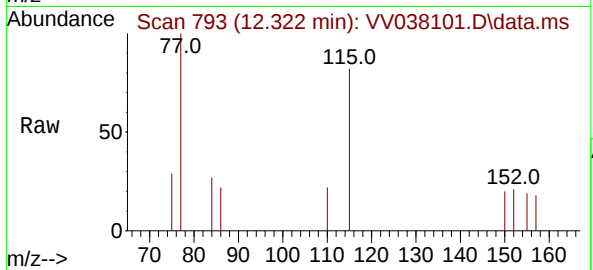

Tgt Ion: 75	Resp:	54
Ion Ratio	Lower	Upper
75	100	
157	64.0	69.4 104.0#
155	65.3	61.3 91.9

